

# Magnetic Resonance Imaging (MRI) Safety



Heather Davis, RT(R), Radiology  
Amy Anderson, RT(R), MR, Radiology

April 2025

## Goal and Objectives

### Goal

This course will enable the learner to provide a safe environment for patients and staff who are in the presence of the MRI scanner.

### Objectives

1. Describe basic knowledge of magnetic fields and their influence on objects near them.
2. Describe the importance of safety when working around the MRI scanner.
3. Identify precautions that should be taken to avoid accidents when working near the MRI scanner.
4. Identify precautions that should be taken when patients have implantable devices or metallic foreign bodies.

## The MRI Magnet

Magnetic resonance imaging (MRI) is a noninvasive, painless medical test that helps physicians diagnose and treat medical conditions by providing views of the inside of the human body.

The MRI uses a powerful magnetic field, radio waves, and a computer to produce detailed three-dimensional pictures of internal body structures.



## The MRI Magnet *(cont.)*

Most people have had some experience with natural magnets and their attractive forces, such as, attaching papers to a refrigerator door.

The MRI scanner is a large magnet (10,000 lbs.) with a tremendously strong magnetic pull. The magnet in the MRI scanner creates a force field which can affect objects that are close to it. As you approach the MRI scanner, the attractive force field increases rapidly.

The strong magnetic field can have adverse effects on patients and staff who are within the scanner's magnetic force field.




## Magnetic Field Hazards

All MRI magnets have a magnetic field that extends into the exam room.

The various distances from the magnet consist of **GAUSS Lines**, which measure the attractive force of the magnet at a certain distance.

As Gauss Line distances decrease, the magnetic field strength increases, until the field is so strong, it can cause any ferromagnetic object\* to have a missile effect.

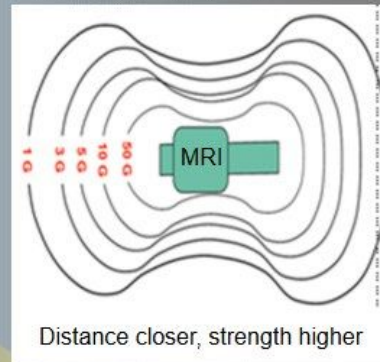

\*An object attracted by a magnet and can become magnetized.

## Magnetic Field Hazards (cont.)

Ferromagnetic metal alloys usually contain iron, nickel, or cobalt. These elements are found in most metal objects.

Examples of ferromagnetic objects:




## Magnetic Field Hazards *(cont.)*

### The Missile Effect

This refers to the capability of the MRI magnetic field to attract a ferromagnetic object into the scanner with considerable force.

It can cause:

- Delayed patient care
- Possible injury to patient or staff
- Possible damage to the MRI scanner
- Approximate cost due to each "missile effect" incident: **\$250,000**



It takes **96 hours** to:

- Turn the magnet off
- Remove the object
- Power back up

The MRI Magnet is Always On!

The MRI Magnet is Always On!

The MRI Magnet is Always On!

## Test Your Knowledge

Which of the following items should you remove from your pockets prior to entering the strong magnetic field of an MRI system?



- Scissors
- Safety pin
- House key
- All of the above

## Magnetic Field Hazards *(cont.)*

MRI staff should ensure that implants are **“MR Conditional”** and should instruct patients to immediately report any burning sensations experienced during the scan.

Displacement and Heating of Surgical Implants:


- Cardiac pacemakers
- Neurostimulators
- Pain control pumps
- Penile implants
- Cochlear implants



## Magnetic Field Hazards (cont.)

Displacement (movement) of these implants may cause a life-threatening situation!

Stents and Aneurysm Clips:

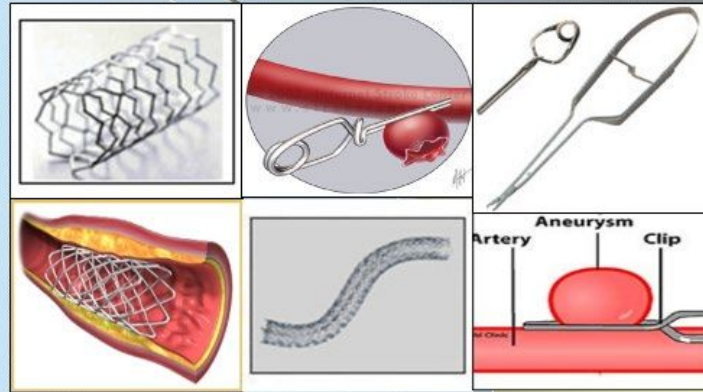


## Magnetic Field Hazards (cont.)

### Electromagnetic Interference with Electronic Devices

Mechanically- or electrically-activated implants may **stop or malfunction** in the presence of the MRI magnetic field.

Patients with pacemakers have died during or shortly after MRI exams due to disruption of pacemaker function by the MRI system.

Hospital staff with pacemakers or other implanted electronic devices could also be affected, if they come within the strong magnetic field of the MRI.

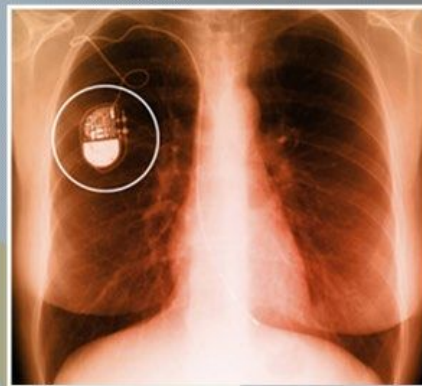

## Magnetic Field Hazards *(cont.)*

All patients with body piercing jewelry must be screened for jewelry removal before they have an MRI scan!

Risks for these patients include:

- Discomfort or painful sensations due to possible displacement of the jewelry.
- Patient burns due to heat generated from the interaction between the jewelry and the electromagnetic fields.




## Magnetic Field Hazards *(cont.)*

All patients with transdermal patches must be screened for patch removal before they have an MRI scan.

Transdermal Patches:

Some patients are now wearing trans-dermal patches for medication delivery.

Many of these patches contain aluminum foil or other metallic components which can cause excessive heating, leading to burns in patients undergoing a MRI scan.



## Magnetic Field Hazards *(cont.)*

All patients with tattoos must be screened before they have an MRI scan.

### Tattoos:

Many patients scheduled for an MRI scan will present with tattoos.

These tattoos will be either cosmetic or decorative and can be located anywhere on the body.

Some of these tattoos will contain ferromagnetic material, which can cause heating, swelling, or burning at the tattoo site.



The MRI Magnet is Always On!

The MRI Magnet is Always On!

The MRI Magnet is Always On!

## Magnetic Field Hazards (cont.)

Pregnancy **All pregnant patients must be screened before they have an MRI scan.**

MR imaging is recognized as a beneficial diagnostic tool to assess a wide range of diseases and conditions that affect pregnant women and their fetuses.

MR imaging in pregnant women should only be performed in cases where the referring physician and radiologist agree that the findings of the MRI has the potential to change or alter the care of the mother or fetus and that the benefit outweighs the risk.

The Policies, Guidelines, and Recommendations for MRI Imaging, Safety, and Patient Management issued by the Safety Committee of the Society for MRI imaging states:



“MRI may be used for pregnant women if other non-ionizing diagnostic imaging is inadequate, or if the MRI provides important information that would otherwise require exposure to ionizing radiation (CT, fluoroscopy, etc.).”



## Summary of MRI Hazards

Hazard	Possible Danger
Body-piercing jewelry	Displacement; Heat
Transdermal skin patches	Burning
Tattoos	Burning
Aneurism clips	Displacement
Stents	Displacement
Cochlear implants	Displacement
Penile implants	Displacement
Pacemakers	Malfunction or Stop

## MRI Patient Safety Labels

Click each label to learn more:



**MRI Safe Equipment Label**  
No Restrictions



**MRI Conditional Equipment Label**  
Equipment needs to be tested prior to use



**MRI Unsafe Equipment Label**  
Equipment is strongly ferromagnetic and must not be used in the scan room


## Thermal Injury Protection

Electrical currents can be induced while in the magnet bore and cause thermal injury.

More tips:

- Cold compresses can be used over heavy tattoos to reduce tissue heating.
- Surface coils should be checked before scanning.
- Unused electrically-conductive materials outside the patient should be removed.

Arms and legs should not cross or touch each other.



The patient's body should not touch the inner bore of the magnet.



## Emergency Shutdown (Quenching)

A loss in superconductivity can result in massive heat gain in the magnet, producing cryogen boil-off and release. This is called “quenching.”

- The resulting damage caused by quenching is costly and time-consuming.
- Emergency quenching should be avoided.
- If extended power loss is expected, the magnetic field can be ramped down to prevent quenching. Backup or temporary power should be available at all times.



## Patient Hearing Protection

- MRI systems can produce a very noisy environment for the patient.
- All patients should be offered hearing protection, especially when using systems which have sound pressures above 99 dB.



## Patients with Claustrophobia - Anxiety - Emotional Distress

- Many patients experience anxiety prior to and during MRI exams. Some may not be able to complete the exam due to claustrophobia.
- It can be helpful to use audio and visual distractions.



## Patients Requiring Immediate Medical Attention

- When a patient needs immediate medical care in the scan room, all responders must have sufficient training in MRI safety.
- This applies to medical/technical staff, as well as police, fire, and security personnel.
- If resuscitation is needed, the patient should be moved from the scanner to a safe area.
- Emergency and disaster plans should be in place and conducted periodically.



## Screening

All **patients** and any **family members** entering the MRI Scanner must be screened by the MRI technologist.

All **ancillary staff** entering the MRI Scanner must verbally be screened by the MRI technologist.

## Screening Patients

All patients must complete the Magnetic Resonance Imaging Information Form\* before they have an MRI scan.

\* These forms are **not** currently used at Grayling Hospital or Otsego Memorial Hospital.

### Outpatient



### MAGNETIC RESONANCE IMAGING (MRI) PATIENT INFORMATION / ASSESSMENT



Patient Legal Name: \_\_\_\_\_  
 (Last) (First) (Middle Initial)

Date of Birth: \_\_\_\_/\_\_\_\_/\_\_\_\_ Age: \_\_\_\_ Height: \_\_\_\_ Weight: \_\_\_\_ (lbs.)

Have you had surgery on the area being scanned today:  Yes  No If yes, when? \_\_\_\_\_

Previous radiology exams on the area being scanned today:  Yes  No

If yes, what type of exam: \_\_\_\_ X-RAY \_\_\_\_ Cat Scan \_\_\_\_ Ultra Sound \_\_\_\_ MRI \_\_\_\_ PET

Briefly describe why your doctor wants this MRI: \_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_

## Screening Patients (cont.)

All patients must complete the Magnetic Resonance Imaging Information Form\* before they have an MRI scan.

\* These forms are not currently used at Otsego Memorial Hospital.

### Inpatient

1 of 3

**MUNSON HEALTHCARE** Form #12254 (06/20)

**RN RADIOLOGY MRI CHECKLIST**

**RN TO COMPLETE WITH PATIENT PRIOR TO MRI**

- Is the MRI questionnaire filled out and signed by the patient?
- Does the patient have any implants?
  - If yes, is the make and model identified?
  - Do you need assistance identifying?
- If the patient is in the ER:

## Screening Patients (cont.)

### Patients with Metallic Foreign Bodies

- All patients with a history of injury by a metallic foreign body must be screened and evaluated before being placed in the magnetic field of an MRI scanner.
- Examples of metallic foreign bodies:
  - ✓ BBs
  - ✓ Bullets
  - ✓ Pellets
  - ✓ Shrapnel
  - ✓ Buckshot
  - ✓ Eye or body metal fragments



## Screening Patients *(cont.)*

### Patients with Implants

- Information that must be supplied by the patient, a family member, or by hospital staff for a patient with an implant includes:
  - ✓ Make and model of implant
  - ✓ Manufacturer of implant
  - ✓ Date of implant insertion
- Medical Alert Cards: Most people who get an implant receive a medical alert card stating whether or not the implant is MRI compatible. These cards should be checked by the MRI technologist.



The MRI Magnet is Always On!

The MRI Magnet is Always On!

The MRI Magnet is Always On!

## Safety Considerations

### Zones of Exclusion

Joint Commission standards require Radiology to have **four zones** of exclusion when performing MRI exams.

Click the buttons to discover the zones.

Reception Desk	Patient Dressing Room	MRI Control Room	MRI Magnet Room
Zone 1: General Public	Zone 2: Unscreened MRI patients	Zone 3: Screened MRI patients and MRI personnel	Zone 4: Screened MRI patients under constant direct supervision or trained MR personnel

## References

Gould, T., & Edmonds, M. (2010, October 25). How MRI works. In *howstuffworks*. Retrieved September 15, 2022, from <https://science.howstuffworks.com/mri.htm>

MR safety. (n.d.). In *American College of Radiology (ACR®)*. Retrieved September 22, 2022, from <https://www.acr.org/Clinical-Resources/Radiology-Safety/MR-Safety>

MR safety. (n.d.). In *The MR Core Research Facility*. Retrieved September 15, 2022, from <https://www.mrc.wayne.edu/safety.htm>

Munson Medical Center Policies and Procedures. (2022, January 3). *MRI safety*. PolicyStat.

Further Questions? Call Heather Davis, Radiology, ext. 57244

# Philips Monitoring System (MUNSON)



## Philips Monitoring System (MUNSON)

### ■ Introduction

#### Central Monitoring System

The Philips Patient Information Center is a regulated medical IT system that:


- Provides continuous monitoring of patient vital signs from admission to discharge.
- Consolidates and communicates vital signs data from monitors and third-party devices to caregivers and to the Electronic Medical Record (EMR) for a complete patient record.
- Supports industry standard interfaces to integrate into existing hospital IT infrastructure and EMR systems while meeting requirements for manageability, serviceability, and security.
- Meets the needs of caregivers on the go by means of remote access to patient vital signs for information anywhere.

Through a combination of advanced alarm management, mobility, and clinical decision support, Philips Patient Monitoring Systems enable reduction of non-actionable alarms, improve workflow efficiency, and facilitate early intervention of patient deterioration to improve patient care and outcomes.

The Information Center software runs on a PC workstation with one or two displays for viewing patient data and accessing clinical applications. A mouse and keyboard are provided for entering and changing patient data and other information. If you position the cursor on a labeled application button and click, the application is immediately displayed on the screen. Note that an on-screen keyboard is not available.

With a touchscreen, you can access patient data by either using the mouse or by touching the item on the screen with your finger or a stylus. The mouse is best for making precise selections and measurements, such as using calipers. The touchscreen is best for actions such as acknowledging alarms, accessing application windows, or recording strips. When using a touchscreen, keep the area free of items that can inadvertently touch the screen. If the touchscreen becomes unavailable for any reason, you can access patient data by using the mouse and keyboard.

The Main Screen displays real-time waves, numerics, and alarms from multiple patients. It can be configured to show up to 64 waves, and contains the following elements:

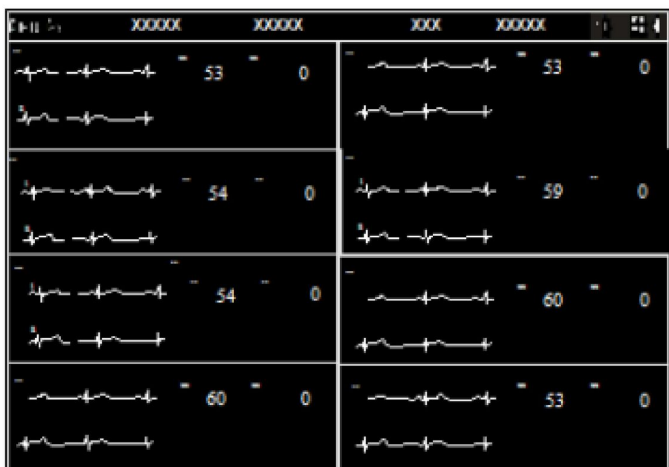

1 Caption Bar

## 2 Patient Sectors



Select the Patient Window button to open the Patient window to Display a real-time view of the current patient's data. You also can choose to do an ECG analysis to view all available ECG leads. The Patient Window provides a real-time view of the patient's waves and numerics. You can view patient data and perform all tasks in the Patient Window. In addition to the waves and numerics, the Patient Window contains the following items:

- The Bed Label Pane - Displays the bed label and ID for the currently selected patient. Select the down arrow to select another patient to view.
- The Print Icon to start a printout of the Patient summary report.
- The Help Icon.
- Alarm message areas – All active alarms and technical alarms display on the top right of the patient window. Status messages are color-coded to indicate the message severity. Orange background indicates high severity. Black background indicates low severity. Select the status message to open System Help in the application window. The Help contains a list of status messages with the possible causes and recommended actions for each message.
- Patient Name - Displays the patient's name. Depending on the length of the complete string and the amount of available space, a minimum number of characters is shown, ending with an ellipsis (...). Three question marks (???) precede the patient's name when there is a problem identifying the patient. For example: Patient data between the Information Center and the bedside does not match. All required information was not entered when the patient was admitted.

Buttons in the sector become visible when you move the cursor into the sector or, if using a touch screen display, when you first touch the sector with a stylus or the tip of your finger. When you place the cursor inside a patient sector, the sector is outlined in an orange border. You can minimize the buttons by moving the cursor into the sector and holding down the **Ctrl** key. While the cursor is inside the sector, the buttons remain minimized until you press the **Ctrl** key again. If you move the cursor out of the active sector and move it back in, the buttons become visible.



Select the Manage Patient icon, which will allow you to:

- Admit, discharge, and transfer patients.
- Enter or update patient demographic information.
- Manage the equipment associated with the patient.
- Temporarily place the bed in standby.
- Enter a temporary transport location, and/or select the patient's equipment to place in standby.
- Export ECG waveform data to a Philips Holter system for analysis.

**To Admit a Patient:** Use one of the following methods:

- Manually enter new patient information in the fields in the **Patient Demographics** section by typing a 1-30 character first and last name in the appropriate fields. You can use the TAB key to move from field to field. You can also admit a new patient by entering the MRN.
- Use the **Find Patient...** option to find a patient who is being monitored in another Information center or who has been recently discharged.

You can then choose the patient's gender from a drop-down list. It will default to Male while performing a 12-lead if not assigned. It will default to Female while measuring STE if not assigned. Specify the patient's birth date by entering it on the calendar. This will update the age field. Enter the patient's height in the appropriate field. This can be in inches or centimeters according to your policy. Enter the Patient's weight using pounds or kilograms according to your policy. Select "Apply" after verifying all information is correct.

Read all confirmation messages and check patient alarms, settings, and paced status when automatic admission, discharge, or transfer is complete.

## **Viewing and Adjusting Waves:**

When the ECG measurement is on, the first wave displayed is the primary ECG wave. The primary wave is always used for ECG analysis. A rhythm status message displays in the upper right corner of the wave, and an arrhythmia status message displays above and in the center of the wave.

Pleth waves on an Efficia monitor are labeled as SpO<sub>2</sub>.

## **Wave Adjustments**

You can adjust waves in the patient sector or Patient Window layout by selecting a wave then selecting one or more options described below.

- Change Wave – Select a wave from the list. You cannot select the primary ECG wave.
- ECG Analysis – Available if you select an ECG wave. Select to access the ECG Analysis application.
- Primary Lead – Available if you select the primary ECG wave. Select the primary led from the list.
- Size up or Size down - Select to increase or decrease the size (gain) of the wave (if available).
- Set up ECG – Available if you select an ECG wave. Select to access the **Measurements** application ECG page, where you can change heart rate limits and asystole thresholds.

**Manually Transferring a Patient to a New Bed:** Transfer data for a patient by performing the following steps:

- Use one of the following methods to open the **Manage Patient** In the sector for the bed that you want to transfer, select the name field or select the **Manage Patient** shortcut button. In the application window task bar, select the **Manage Patient** button.
- Select the .. button. The **Transfer Patient** dialog box displays a list of available beds in the institutions and units.
- To transfer this patient to another bed within this unit, select the bed from the list of beds in your unit. To transfer this patient to a bed in another unit, first select the unit name, then select a bed from the list.
- Specify whether to clear the sector (remove the bed from the sector) upon transfer by selecting or clearing the **Clear Sector** check box. The system can be configured so that the check box is selected by default. Depending on your unit practices, you may want to clear the check box so the sector is not cleared and the equipment remains assigned to the sector.
- Select "OK".
- Confirm the transfer by selecting the orange "TRANSFER" button.

**To Discharge a Patient:** Use one of the following methods to discharge a patient.

- Manually discharge a patient in the **Manage Patient** application.
- Discharge a patient directly from the hospital information system or bed management system.

## **Considerations**

Before discharging a patient, note the following:

- Discharging the patient at the Information Center also discharges the patient from the bedside monitor. All monitor and MMS settings (including arrhythmia settings) reset to their defaults.
- When you discharge a patient, the Information Center saves the patient data for all admitted patients. The system stores seven days of data and purges the stored data seven days after discharge.

You can search discharged patient data without readmitting for up to seven days.

- If you readmit a patient, the discharge data is overwritten by new monitoring data as it occurs, and you will only see the full disclosure amount of data.
- Monitoring devices may be set up with predefined configurations called *profiles*. When you discharge a patient, the profile reverts to the default profile configured for the device. Refer to your monitoring device documentation for details. When

you discharge an admitted patient at the Patient Monitor, the Information Center discharges the patient and saves the data.

- *Important* — For MRx monitors, turning off the bedside monitor for more than 10 seconds discharges the patient at the MRx monitor and resets defaults, but it does not discharge the patient from the Information Center; the patient is still admitted at the Information Center. It is important to discharge the patient before turning the monitor off to avoid data being associated with the wrong patient.
- Patients that are discharged while the Information Center is in Local/Disconnected mode will be synchronized upon connection to the primary server.

## **Warning**

Read all confirmation messages and check patient alarms, settings, and paced status when automatic admission, discharge, or transfer is complete.

## **Measuring ECG:**

The electrocardiogram (ECG) measures the electrical activity of the heart and displays it on the Information Center as a waveform and a numeric. In order to compare measured ECG signals, the electrodes are placed in standardized positions, forming "leads". To obtain ECG signals optimized for use in diagnosis and patient management in different care environments, different lead placements can be used.

## **Selecting the Primary and Secondary ECG Leads**

The telemetry device or patient monitor uses the primary and secondary lead selected at the Information Center to compute HR and to analyze and detect cardiac arrhythmias.

You should choose a primary and (if using multi-lead monitoring) secondary lead that have the following characteristics:

- the QRS complex should be either completely above or below the baseline and it should not be biphasic
- the QRS complex should be tall and narrow
- the T-wave should be less than 1/3 the R-wave height
- the P-wave should be less than 1/5 the R-wave height

## **Documenting Patient Events**

Documentation of patient events and procedures is a necessary element of patient care. You can print reports from the PIC iX to paper, electronically via PDF, or both.

## **Create a Saved Strip**

You can create a saved strip with the PIC iX electronic caliper (eCaliper) measurements and comments in any strip tile in Alarm Review, General Review, or specialty review applications.

*Note* —You must have Full Permission Access to annotate and save a strip to the database.

- Select the strip that you want to annotate.
- Select the Annotate icon. The Saved strip dialog box opens. You can move the dialog box as needed.
- Select a label from the drop-down list to add labels. This field can be customized as needed in Alarm Review.
- Enter text in the second field, up to 30 characters. This value displays in the Comment field for the strip.
- Add eCaliper measurements. Consider changing the wave speed to 50 mm/sec. (Select the speed on the bottom right of the strip, then select a speed from the list.) Click and drag in the strip to and from the desired location in the wave. The measurement is displayed between the vertical lines. In the dialog box, click the measurement label to add the measured value. *Note* — Double-click the measurement to see the caliper bars at any time.
- Select another strip and repeat these steps as needed.
- When you are done, select Save. The measurements are saved to the strip.

## Reviewing ECG Waves

Depending on the number of ECG leads and licensing, 3 to 12 waves are available for review. These waves can be reviewed with the other data tiles, such as with events and alarms.

### Alarms:

**Quickly Viewing Target Events** - When reviewing patient data, it is often helpful to quickly view specific types of alarms or events.


**Fast Alarm Review** - Select either the Acknowledge key, or the alarm banner in the sector to see alarming waves prior to being available in other applications. Alarm strips can be printed, annotated, or discarded. If you are using secondary notifications, such as with Philips CareEvent, you can manually page an alarm from this application.

*Note* — The Silence key is called the Acknowledge key.

## Alarm Review

Alarm Review always opens with the most recent alarm strip. To review alarms, open Alarm Review from the Review sector button, if configured, or you can open Alarm Review from the main Setup menu or from the Review application menu in any open application. Use the toggle icon to switch between the three different tiles. The tile you prefer can be set up as a default on each host.

- **Tabular** tile – shows a detailed strip with multiple waves and a tabular list of alarms. Use the up and down arrow keys to quickly view alarm strips. This is the factory default tile.
- **Compressed** tile – shows 30 seconds of compressed waves for all strips.
- **Strip Window** tile – a combination of Compressed and Strip tiles.

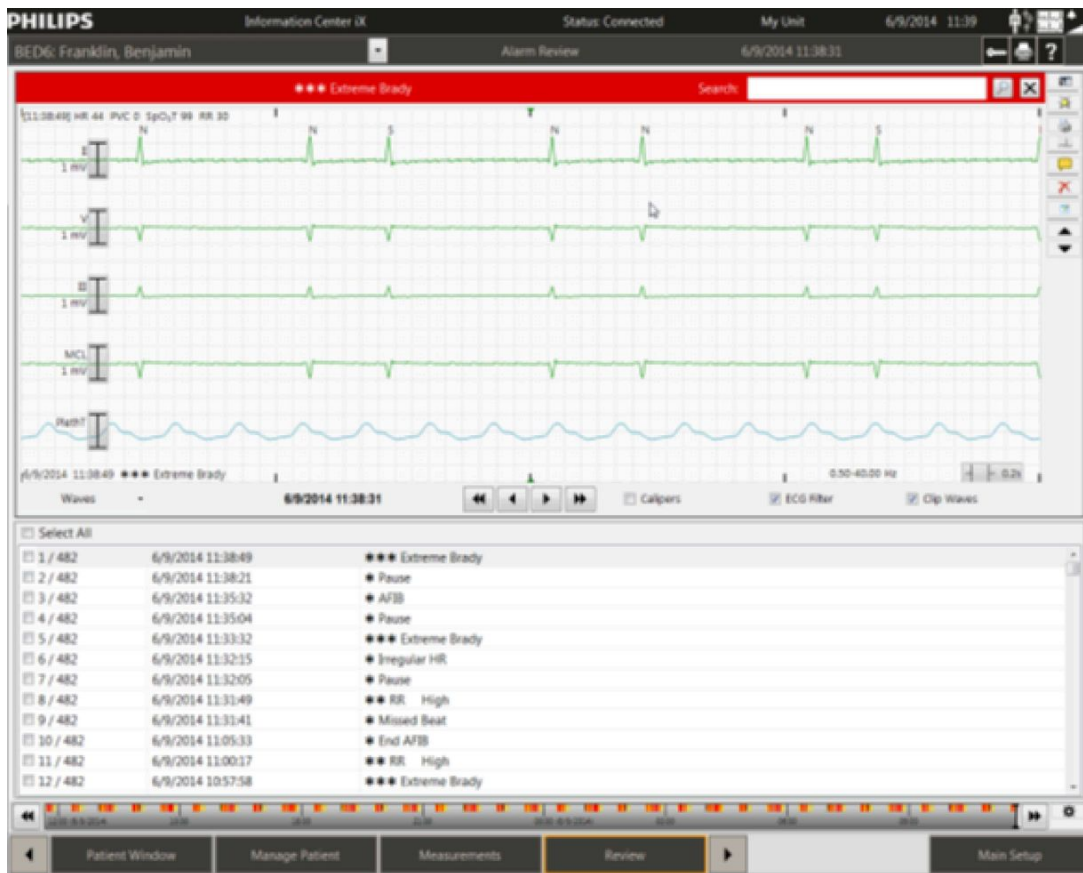

## Reviewing Alarms and Events in Other Applications

Within the factory default review applications (as well as custom applications that were created for your unit), there is a data type called the Event tile. You can use the Event tile to review alarms with other associated data, such as compressed wave storage or graphical trends. Arrhythmia events are also shown, even when a specific alarm is off, such as for yellow level ventricular alarms. The length of the colored box indicates the duration of the event.

- Open the review application. If opened from Alarm Review, the time focus is the selected alarm. If opened from another application, it opens at the current time minus the one minute for storage.
- The Event tile is highlighted below. Note the displayed number of events shown on the right. Alarms are shown with the corresponding color, and arrhythmia events are shown in cyan.



- Clear the check box next to the events you do not want to see. If licensed, specific events can be customized for each review application.
- Move the cursor over any alarm or event to see text that contains the details.
- Select the event to examine its associated waves, trends, and numerics.
- Use the arrow keys in the middle of the tile to quickly navigate to next or previous events.



Alarms off. Displays next to the numeric when alarms are turned off for the numeric.



Pause Alarms (Red and/or yellow). **PRESS THIS BUTTON AGAIN TO RESUME ALARMS!**



Acknowledge/Review Button. Turns off the alarm sound and the sector background changes from blue to black.



Volume icon. Select to adjust the alarm volume.

Physiological alarms are red and yellow alarms. A red alarm indicates a high priority patient alarm such as a potentially life-threatening situation (for example, asystole). A yellow alarm indicates a lower priority physiological alarm (for example, a respiration alarm limit violation). Additionally, there are short yellow alarms, most of which are specific to arrhythmia-related patient conditions (for example, ventricular bigeminy). Alarm message areas. All active alarms and technical alarms/INOPs display on the top right of the patient sector. A RED warning alerts you to a potential serious outcome, adverse event or safety hazard. Failure to observe a warning may result in death or serious injury to the user or patient. A YELLOW caution alerts you to where special care is necessary for the safe and effective use of the

product. Failure to observe a caution may result in minor or moderate personal injury or damage to the product or other property, and possibly in a remote risk of more serious injury. Technical alarms, or INOPs indicate that the monitoring device cannot measure or detect alarm conditions reliably. If a technical alarm interrupts monitoring and alarm detection (for example, LEADS OFF), the numeric is replaced by a question mark in the sector and Patient Window, and an audible indicator sounds. Technical alarms without this audible indicator indicate that there may be a problem with the reliability of the data, but that monitoring is not interrupted. Most technical alarms are light blue, however there are a small number of technical alarms that are always yellow or red to indicate a severity corresponding to red and yellow alarms.

There can be only one alarm sound annunciating at the Information Center at one time.

- If there is an unacknowledged red level alarm in the presence of any other level alarm, the sound for the red alarm annunciates.
- If there is no unacknowledged red level alarm condition and there is an unacknowledged long yellow alarm in the presence of any other yellow technical alarm (acknowledged or unacknowledged) the sound for the long yellow alarm annunciates.
- If there is no unacknowledged red level alarm or long yellow level alarm condition and there is an arrhythmia or nurse call event, the short yellow (\*) alarm sound annunciates.
- If there are no unacknowledged red or long/short yellow alarm conditions and there is any bed with an unacknowledged technical alarm condition, the sound for the technical alarm annunciates.
- If multiple sectors are in alarm, once the highest level alarm is acknowledged in a sector the next highest alarm annunciates.
- An alarm tone indicates the alarm type. There is no sound for soft INOPs/technical alarms.

### **Other Buttons and Icons:**



**Battery icon.** If there is at least one battery-operated device assigned to this patient, the battery icon indicates the device with the least amount of battery strength. Move your cursor over the icon to view a list of equipment for this patient sorted from the lowest to highest battery charge. The battery icon has five levels: approximately 100% to 80%, 80% to 60%, 60% to 40%, 40% to 20%, or -Replace Battery strength. The number of segments indicates the approximate power level.



**Help icon.** Select to view the online Help application. The Help application is always available and provides context-specific information on using the Information Center applications.






**Manage Patient icon.** Available in sectors not currently monitoring a patient. Select the icon to access the **Manage Patient** application where you can assign a monitoring device.

**The Measurements Button:** Provides access to the **Measurements** application, which allows you to:

- Change alarm limits for a patient.
- Turn specific alarms on or off for a patient.
- Adjust measurement settings within a profile.
- Set up telemetry devices.
- Designate which alarms will generate a recording or report or initiate a page.
- View or print an Alarm Summary.
- Configure criteria to trigger alarm advisor notifications.
- View active notifications.

Your choices in the application depend on how your unit is set up and the equipment assigned to the patient.


**Paced Mode icon.** Indicates the patient's current paced status.

-  On – The icon is white when **Paced Mode** is turned on.
-  Off – The icon is green with an X over it when **Paced Mode** is turned off.
-  Unconfirmed – A red question mark displays over the icon when the patient's paced mode is unknown or in conflict.

The pacer spike color is always white unless the ECG wave is white. If the ECG wave is white, then the pacer spike color is green. Pacer spikes may be configured to display with fixed amplitude for increased visibility.

*Important* — If **Paced Mode** is set to **Unconfirmed**, the ST/AR algorithm acts as though **Paced mode** is turned on. Select the icon to display a menu where you can turn **Paced Mode** on or off.

**Warning** - If the patient has a pacemaker, **Paced Mode** must be turned on, enabling the ST/AR algorithm to detect and reject pace pulses (spikes) from the HR count. Otherwise, pace pulses could be detected as beats and the monitor may not alarm for an asystole condition. If the patient does not have a pacemaker, turn **Paced Mode** off to allow the ST/AR algorithm to work most effectively.



**Print/record Icon.** Depending on your system setup, select this icon to do the following:

- **Record All** — make a delayed recording for all sectors that currently have patient data.
- **Print All** — print a strip for all patients in the unit.
- **Save Strips** — create saved strips for all patients in the unit.

If you select this icon, a message asks you to confirm that you want to proceed with the action. Select **Yes** to confirm. Your system may be set up to just record, record and save a strip, or to just save a delayed strip.

### Resuscitation Status Icons:



Do Not Resuscitate. Resuscitation icon. Indicates the patient's current resuscitation status.




Modified. The icon is solid white when the patient's resuscitation status is set to **DNR** (Do Not Resuscitate). The icon is a white outline when the patient's status is set to **Modified**. The icon does not display if the patient's resuscitation status is set to **Full**. Select the icon to access the **Manage Patient** application where you can change the resuscitation status.

### Prior Data:

Patient data can be stored up to 7 days for each patient of Retrospective Review at Central Station. Data stored upon discharge, or from another unit with a transfer, will be shown separately from current data.

« SCROLL »

- A Prior Data icon shows in the review applications. Selecting it opens a menu of prior encounters.

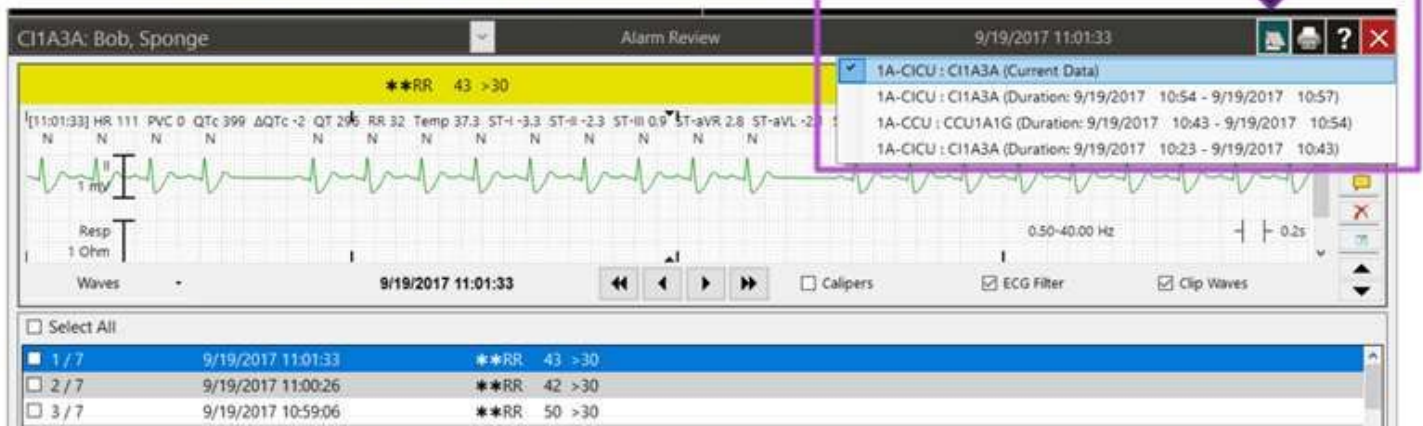

Once you are into this window –

- The Information Bar at the top turns teal green (states 'Prior Data')
- The only smart key on the bottom task bar will be 'Review'
- Main Screen button becomes 'Current Unit'
- To close the application, use the red X in the upper right or choose the Current Unit button

« SCROLL »



## References:

- MX Series QR Codes
- Central Monitoring Station PICiX
  - IFU\_-\_PIC\_iX\_Rel\_C.03\_-\_English.pdf- Central station user manual
  - PIICiX Rev C.03 Patient Data Review
- MX40 Telemetry box
  - the MX40 IFU manual link
  - the MX40 quick card reference
- MX400 Large Mounted Monitor
  - IFU MX400-800\_IVPM\_N0x)Mar2019.pdf User manual
- Invasive pressure Guide
  - Invasive Pressure PDF
- Capnography
  - Capnography Application Guide

## ■ Notes

### MX Series QR Codes

 Scan the QR Codes with a smart phone camera for Quick access to Philips YouTube videos for the Philips MX Series Patient Monitor



**MX Series-Front Hardware (2 min)**






**MX Series-Rear Hardware (3 min)**



[View image in PDF format.](#)

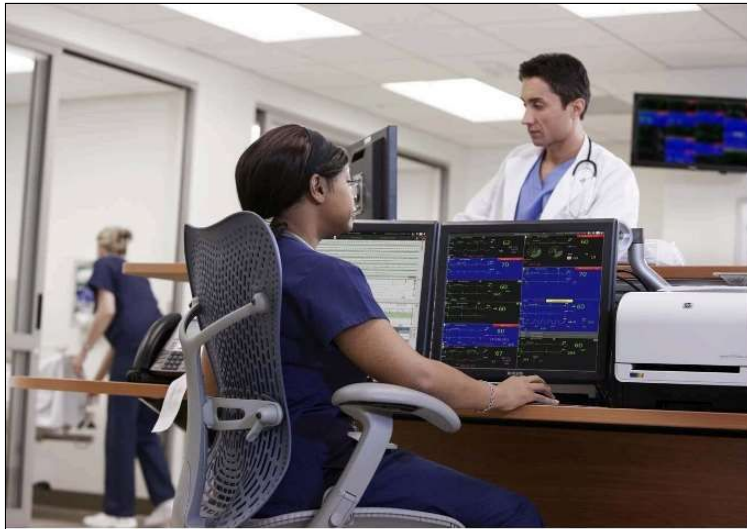


## Patient Information Center iX

Instructions for Use

Release C.03

**PHILIPS**

[View image in PDF format.](#)

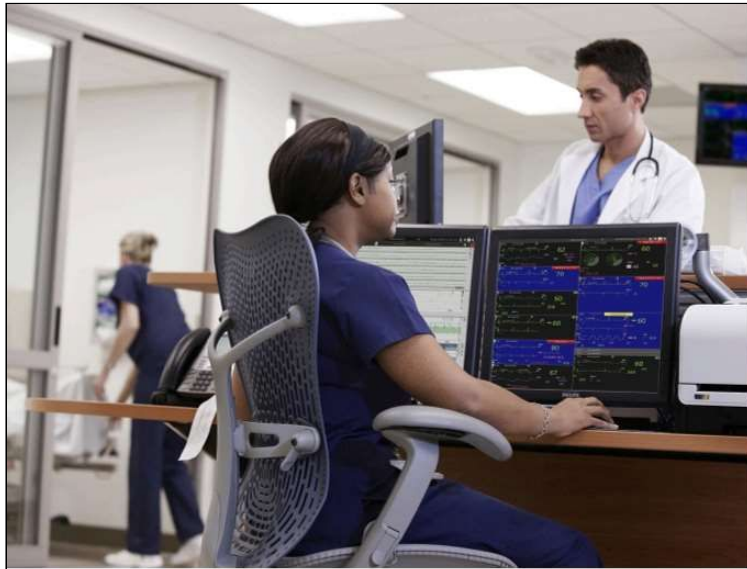

## PIC iX Patient Data Review

Quick Guide

Release C.02/C.03

[View image in PDF format.](#)

Car Seat Quick Guide

## Car Seat Assessment Record (CAR) Quick Guide

1. Place baby in car seat.

2. Change Screen to **CAR SEAT TEST**.



3. Touch SmartKey – **START CAR**.

4. Select amount of time for Test Duration  
(based on hospital protocol).



5. Touch **CONFIRM** key.

\*\*\*CAR is now in progress\*\*\*  
Monitoring is continued during CAR.

6. If at any time during CAR you need to  
exit or stop – press the SmartKey **STOP  
CAR** and **CONFIRM**.

At any time you can also switch back to  
your default monitoring screen by  
touching **Change Screen**, then touch  
the back arrow at the top of that menu.  
*CAR will continue to run in the back  
ground.*

7. When CAR is complete, the countdown  
timer (to the far right in the CAR Screen)  
will turn **RED**.



[View image in PDF format.](#)

# Preparing A Patient For Surgery



Molly Gallagher, BSN, RN, CAPA  
Jeannette Reynolds, MSN, BBA, RN, CPAN

October 2025



## Goal and Objectives

Document was last saved: Just now

### Goal:

This course provides information on the Preprocedure checklist and provides rationale on inpatient preparation for surgery or a procedure.

### Objectives:

1. Accurately complete the Preprocedure checklist for a patient going to the Operating Room (OR), Medical Procedure Room (MPR), or Interventional Radiology (IR).
2. Correctly perform the pre-surgical hygiene elements when preparing a patient for surgery or a procedure.
3. Explain the importance of the Beta Blocker regimen during the peri-operative period.

# Preprocedure Checklist

- Begin the Preprocedure checklist as soon as you know the patient is going to surgery - ideally the day before surgery.
- Must be completed for every patient going to the OR, MPR, or IR for surgery or procedure.
- With the patient's chart open, click AdHoc.
- Select preprocedure checklist.
- The acute care nurse will complete the first 4 pages of the powerform.

# Preprocedure Checklist (cont.)

(Hover over highlighted box.)

**Complete these four pages.**

Preprocedure Checklist
Preprocedure Checklist

**STOP HERE**

**Procedure Location**

Bodis   
  Emergency department   
  Operating room   
  MPR/SFR   
  OR operating room  
 Catheterization lab   
  GI lab   
  Radiology   
  Cardiac diagnostic suite   
  Other

**Last Fluid Intake**

no pre/procc [ ] [ ]

**Last Fluid Intake Amount**

[ ] mL

**Last Void**

no pre/procc [ ] [ ]

**Last Food Intake**

no pre/procc [ ] [ ]

**Last Food Intake Type**

Clay liquid diet  
 Full liquid (other than breastmilk)  
 Solid food

**Carbohydrate Loading**

Yes  
 No

**Patient Preparation**

	Yes	No	N/A	Comment
Makeup removed				
Nails cleaned				
Chlorhexidine showers or bath completed				
Wearing patient gown				
Jewelry removed				
Bowel prep complete				
Oral care complete				
Surgical Clipping, Pre-Up				
Nasal antiseptic				
Mupirocin complete				
Undergarments removed				
Hairpins/hair pieces removed				
Albuterol MDI or nebulizes				

Has patient ever had a reaction to jewelry, clothing snaps, or other items containing metal?

Yes (if not on schedule, notify physician)  
 No

**Right click to view/print Refusal to Remove Jewelry Form**

[ ]

**Right click to view preprocedure policies**

Progress  Page 4 of 22

# Preprocedure Checklist (cont.)

Preprocedure Checklist - SIMS, CLAIRE

Performed on: 01/30/2025 12:50 EST

## Perioperative Protocols

**Patient Safety**

	Yes	No	Comment
Allergy band on and verified			
ID band on and verified			
Limb alert band on and verified			
DNR/DNI band on and verified			
Current ECG in medical record			
Current H&P in medical record			
Relevant Images in Medical Record			
Review of Labs			
Site verified by patient/family			
Site verified by RN			
Site verified/checked by Provider			
Siderails up/wheels locked			
Alarms on and set appropriately			
Call Light Within Reach, Pre-Op			
Antibiotic to OR, Pre-Op			
TED hose/knee			
TED hose/High			
SCD(s)			
Code Status During and/or after a Procedure Form on chart			
Sleep apnea education given			
Hyperglycemia education given (MMC only)			

**Preprocedure Status**

Right click in box to view/print  
Retrieved Patient of Preprocedure Test

**Preprocedure Tests**

	Yes	No	NA	Comment
Anesthesia consent signed				
Site Consent signed				
Procedure consent signed				
Site/Procedure consent from signed (MMC only)				
Other Consent				

Additional Information

Right click in box to view Code Status During and/or after a Procedure Form

Progress  Page 5 of 22

# Nursing - Careset Orders

Search: nursing | Type: Acute Care

- Nursing - A2 Amiodarone Protocol
- Nursing - A2 Digoxin Protocol
- CA Nursing - A2 High Intensity Insulin Drip
- GR Nursing - Constipation Prevention - bisacodyl (Dulcolax)
- MH Nursing - Constipation Prevention - Miralax
- KM Nursing - CRRT KPhos ORAL Electrolyte Replacement
- PO Nursing - CRRT Magnesium IVPB Electrolyte Replacement
- AD Nursing - CRRT NaPhos IV Electrolyte Replacement
- Ca Nursing - Dialysis Care Set
- Ca Nursing - DKA Electrolyte Replacement
- Co Nursing - Flumazenil (Romazicon) Protocol
- CT Nursing - Hyponatremia Reference Test
- Food Nursing - Hypothermia Electrolyte Replacement Protocol
- Pat Nursing - ICU High Intensity Insulin Drip
- Pat Nursing - Inpt Pre-Procedure/Pre-Op Prep Checklist Orders

Enter to Search

Component	Order Details
Bath	qShift, other (specify)
NPO	1/30/2025 12:41 PM EST, NPO
IV Start (Autopage to IV Therapy)	IV patient & gauge appropriate per protocol
Type and Screen	Blood, Routine
Pregnancy Test Urine	Urine, Routine, ONCE
Electrocardiogram - M	Routine, per protocol
Surgery Scheduled for 2 days	
Note: If surgery scheduled is scheduled for more than 2 days into the future the Chlorhexidine Bath Tasks must be rescheduled to the appropriate dates and times.	
Chlorhexidine Bath - Chin to Toe Task	T:1900, Give chlorhexidine bath
Chlorhexidine Bath - Chin to Toe Task	T+1:1900, Give chlorhexidine bath
Chlorhexidine Bath - Chin to Toe Task	T+2:0600, Give chlorhexidine bath

- Order your careset for Nursing - Inpt Preprocedure/Pre-Op Prep Checklist. Enter the careset as a 'Nurse per Protocol' (exception for patients scheduled in Maternity OR).
- Adjust the dates of CHG baths and nasal decolonization to correlate with day of surgery.
- Everything you do to help prepare the patient prior to their arrival in pre-op benefits the patient and prevents delays in surgery start times.

## Treatment Decision Form

- Check code status in PowerChart.
- If the patient is anything except a full code, print a Treatment Decision Form (form #4511) and page the surgeon to complete it.
- Patients going to the operating room **do not** automatically become full codes. A Treatment Decision Form must be completed prior to surgery and will include a date/time to resume patient's preprocedure code status.

1 of 1

MUNSON HEALTHCARE

Form 4511 (08/24)

4511

CODE STATUS DURING AND/OR AFTER A PROCEDURE

Patient Name: \_\_\_\_\_ Date of Birth: \_\_\_\_\_

Surgeon Name: \_\_\_\_\_ Procedure: \_\_\_\_\_

Options: \_\_\_\_\_

Progress  Page 7 of 22

## History and Physical (H&P)


- For all surgical or invasive procedures involving anesthesia or sedation, a valid H&P must be on the patient chart prior to start of the procedure. A valid H&P must have been completed within 30 days (not 31 or more days prior to admission or procedure).
- The surgeon must document in the patient's electronic record (H&P, consult, or progress note) the planned course of action and applicable side of the procedure, if warranted.
  - Writing an order is NOT acceptable as the surgical plan.
- In emergency cases, where completion of an H&P is not feasible, the surgeon should make a notation of relevant history and physical findings in the patient's progress notes, if time allows.

# Informed Consent

- Informed consent is a process of communication between a provider and patient to reach an agreement or permission to perform a procedure. The patient (or designee) signature on the form confirms that a provider has:
  - Reviewed the procedure.
  - Discussed the risks, benefits, or alternatives.
  - Answered all the patient or designee questions.
- The informed consent process could occur on the inpatient floor or at the site of the procedure.
- The patient and the provider performing the procedure will both sign the form (#0303) "Confirmation of Informed Consent for Procedure" (often referred to as CIC) ideally at the time of the informed consent discussion. The form must be signed prior to performing an invasive procedure.
- The signature of the provider performing the procedure **is required** on the form confirming the informed consent process has been completed.
- Consents are **valid for 90 days**.

# Confirmation of Informed Consent for Procedure

1 of 2

 **MUNSON HEALTHCARE**

Form 0303 (03/10/23) Page 1 of 2

**CONFIRMATION OF INFORMED CONSENT FOR PROCEDURE**

You are receiving health care at a facility that is part of Munson Healthcare.  
Munson Healthcare includes the following:

<input type="checkbox"/> Kalkaska Memorial Health Center	<input type="checkbox"/> Munson Healthcare Grayling Hospital	<input type="checkbox"/> Munson Home Health
<input type="checkbox"/> Munson Healthcare Cadillac Hospital	<input type="checkbox"/> Munson Healthcare Manistee Hospital	<input type="checkbox"/> Munson Medical Center
<input type="checkbox"/> Munson Healthcare Charlevoix Hospital	<input type="checkbox"/> Munson Healthcare Otsego Memorial Hospital	<input type="checkbox"/> Paul Oliver Memorial Hospital

You have the right, as a patient, to be informed about your condition and the recommended surgical, medical, or diagnostic procedure to be performed, so that you may make a decision to undergo the procedure with knowledge of the risks, benefits and alternatives. This disclosure of possible risks is not meant to scare or alarm you; it is simply an effort to make you better informed so you can give, or withhold, your consent for the proposed procedure.

**The procedure, treatment, or therapy (Procedure) is:**

I consent to the performance of the procedure named above, by \_\_\_\_\_  
Physician/Provider Name

I know that my provider may ask other healthcare providers to help with the Procedure, which may include other physicians, or other appropriate providers, and my provider has specifically identified any other providers who are likely to assist and/or perform important aspects of the Procedure. I understand that resident physicians, healthcare professionals, and healthcare students may be present to

## Informed Consent Process - Nurse's Responsibility

The nurse serves an important role in the process to optimize patient care and workflow.

- Review the provider's order and electronic record for the planned operative procedure.
- The RN may enter the procedure on the consent form using no abbreviations, or if available, use the procedure-specific consent form.
  - If needed, clarify any abbreviations, illegible or unusual order, and any discrepancies with the provider performing the procedure.
- Confirm the performing provider and patient have both signed, dated, and timed the CIC.
  - If the informed consent discussion occurred with the provider, but the provider did not have the patient sign the form at the time of the discussion, **nursing personnel may facilitate signature of the patient or the designee ONLY in situations where the patient or designee has no questions.**
- Confirm the form is placed in the patient's chart and travels with the patient to the procedural area. If there is no provider or patient signature, inform the pre-procedure staff during hand-off communication.
- The form may be sent to preop holding with only the patient's signature.

## Checklist Components



### Lab Tests

- Check all current lab values and report any abnormal findings to the surgeon.
- Obtain a urine pregnancy test (per Pre and Post Surgical/Procedural Adult Protocols) on all females between menarche and menopause. Women who have had tubal ligation still need a pregnancy test. Women who have had hysterectomies do not.
- Notify the pre-op RN of abnormal lab findings during handoff report.

## Checklist Components



### ECG Prior to Surgery?

#### When:

- There needs to be a normal ECG on the chart from the last year, or the last 6 months if the last ECG was abnormal and patient is stable.
- If using a paper ECG from another facility, it needs to be verified and signed.

#### Who:

- Any patient with a history of a previous MI, angina, arrhythmia, renal failure, medication-dependent diabetes, or CVA.
- Any patient 45 years or older with a history of hypertension or history of  $\geq$  one pack per day smoker.
- All patients 45 years or older having major vascular, intra-abdominal, thoracic, neurological, or orthopedic surgery.

## Checklist Components



### IV Access

- Ensure a patent large bore IV. Refer to Pre and Post Surgical/Procedural Adult Protocols for catheter size required based on the type of surgery.
- If the patient has Heparin infusing, follow the physician orders regarding continuation/discontinuation.
- Discuss with the pre-op RN during handoff report if the patient's IV infusions should be discontinued prior to sending the patient to the peri-operative area.

## Checklist Components



### NPO

- NPO except clear liquids and medications after midnight.
- Stop clear liquids 4 hours before scheduled surgery time.
- If the surgeon's NPO orders conflict with the Pre-Procedure Nothing By Mouth Policy, page the anesthesiologist for clarification.
- Sips of water with meds are ok.

## Pre-Surgical Hygiene

Prior to the pre-surgical bathing:

- **Remove all body jewelry** (including wedding bands).
- Remove hair clips, pins, rubber bands, etc.
- Remove body piercings.
- Remove makeup and nail polish.



Patient who did not remove ring prior to going into OR.

## Pre-Surgical Hygiene *(cont.)*

The patient should have a total of three (3) chlorhexidine gluconate (CHG) baths **if required**:

- Two nights before surgery
- The night before surgery
- The morning of surgery

Example: If the patient's surgery is on Tuesday, bathe with CHG on Sunday night, Monday night, and Tuesday morning.

### **What if the patient is admitted the night before surgery?**

You must ensure two (2) CHG baths are completed:

- The night the patient was admitted
- The morning of surgery

## How to Give a CHG Bath

- Wash the entire body (from neck down) with CHG.
  - Cleanse groin area (avoid CHG on mucous membranes).
- Avoid scrubbing the skin too hard with CHG.
- Do **not** use regular soap after the CHG.
- Do **not** rinse the CHG off of the skin.
- Place the patient in a clean gown after the CHG bath (all clothing, including underwear, should be removed).
- Place clean linens on the bed after the CHG bath.

## Pre-Surgical Hygiene *(cont.)*

### Two nights before surgery:

- Give a soap and water bath **prior** to the first CHG prep bath.
- Shampoo hair with regular shampoo.
- Wash face with regular soap/cleanser.
- After the soap and water bath, give the first CHG bath, using either the wipes or the liquid.

### The night before surgery:

- Wash face with regular soap or cleanser.
- Give the second CHG bath in the same manner as the previous night.
- Brush teeth and use mouth rinse.

## Day of Surgery Preparation

- Use the Preprocedure checklist.
- Complete the 3<sup>rd</sup> CHG (last) bath. Place a clean hospital gown on the patient.
  - Clean under finger nails.
  - Confirm oral care is completed.
  - Encourage the patient to void prior to sending to pre-op.
    - Bathroom availability is limited in pre-op.
  - Remove the patient's underwear.
  - Inform the pre-op RN when medication patches are left on the patient.
- Complete nasal decolonization, if required.
- Document vital signs prior to transfer.
  - Report abnormal findings to the pre-op RN.
- Send the patient with dentures, glasses, and hearing aids.
- Call hand-off report to the pre-op RN.

## Obstructive Sleep Apnea

- Communicate with the pre-op RN if your patient uses a CPAP or BiPAP and discuss if the device should be sent with the patient to the perioperative area.
- Ensure settings are documented, so that the machine can be used accurately postoperatively.

## Antibiotics

- The surgeon or a covering physician shall write specific orders for all patients requiring prophylactic pre-operative antibiotics.
- Confirm an order for preoperative antibiotics is placed in PowerChart by the surgeon or covering provider.
  - Pre-op antibiotics should be administered by the pre-op nurse or anesthesia provider to ensure they are administered within one hour prior to the incision window.
- If the patient is on oral antibiotics, give prior to the patient going to pre-op.
- Ensure **scheduled antibiotics** are given as ordered.
- If a scheduled antibiotic is due during the perioperative period, please send it to OR with the patient.

## Beta Blockers

Patients on a beta blocker at home **should receive their beta blocker** during the perioperative period (24 hours prior to surgery through discharge from PACU).

- Stress associated with surgery increases heart rate, myocardial contractility, and myocardial oxygen demand, putting the patient at risk for an acute myocardial infarction (AMI).
- Beta blockers offer cardioprotection for patients with a history of MI and hypertension. They diminish the effects of epinephrine and other stress hormones.
- An MI during surgery results in a nine-fold increase in unstable angina, MI, and cardiac death in the post-op period.
- If the patient's heart rate is greater than 50 and the systolic blood pressure is greater than 100, administer and document beta blocker in PowerChart.
- If held or stopped for a specific reason, **it must be documented**. This also applies to the perioperative period. Communicate this to the pre-op RN during handoff.
- NPO does **not** mean the patient should not receive their beta blocker. If in doubt, clarify with the surgeon and document who ordered the hold and why it is being held.

## Miscellaneous Medications

### Aspirin (ASA)

If the patient has a cardiac stent and takes a daily 81mg dose of ASA at home, they must have their ASA dose within 24 hours of surgery start time. There are rare instances where the bleeding risk outweighs the benefits and a surgeon may order the ASA be held.

- If the patient is having a neurosurgery procedure, confirm with surgeon prior to administering aspirin.

### Anticoagulants/Anti-platelet medications

- Most anticoagulants will need to be held for invasive procedures/surgery.
- Verify the surgeon's order if anticoagulants are to be held or continued. If no order is present addressing the patient's anticoagulation status, page the performing provider.

### Other medications

Medications such as anti-seizure, Parkinsons, anti-rejection, and chronic pain, should be continued, if ordered.

Please call pre-op holding and ask to speak with the charge nurse if you are unsure about giving a medication.

## References

### Munson Medical Center Policies and Procedures

- Surgical Antibiotic Prophylaxis
- Pre-Procedure Nothing by Mouth Policy
- Ensuring H&Ps are Present Before Surgery/Invasive Procedure
- Skin Preparation of the Surgical Patient
- Jewelry Removal Prior to Surgery
- Pre and Post Surgical/Procedural Adult Protocols
- Plan of Care – Nursing Process in the OR
- Inpatient Pre-Procedure/Pre-Op Checklist and Patient Preparation

### Munson Healthcare Policies and Procedures

- Informed Consent - Diagnostic or Therapeutic Procedures and Treatments

# Overview of Procedural Sedation

Amy Krug, BSN, RN, CGRN  
Lisa Lord, MSN, RN, CNOR  
Jeannette Reynolds, MSN, BBA, RN, CPAN

October 2023



## Goal and Objective

### Goal

This course will ensure standardized practice for delivering sedation/analgesia during diagnostic and therapeutic procedures performed outside of the operating room, according to MHC policy. The ultimate outcome is to provide for the safety of our patients during sedation.

### Objective

After completing this course, the participant will be able to identify the four levels of sedation.


## Exclusion List: Non-Procedural Sedation

The sedation policy and this education module **do not apply** when analgesics or sedative agents are given for the following:

- Pain management (analgesics given by **any** route).
- Minimal sedation (anxiolysis).
- Sedation during emergent medical care in an unstable patient.
- Sedation during ongoing ventilation therapy.
- Sedation for end of life/palliative care.
- Treatment of medical conditions such as delirium, alcohol withdrawal, traumatic brain injury, etc.

## Four Levels of Sedation

In order to provide safe and effective care for patients receiving sedation, it is imperative that health care providers understand the four levels of sedation:

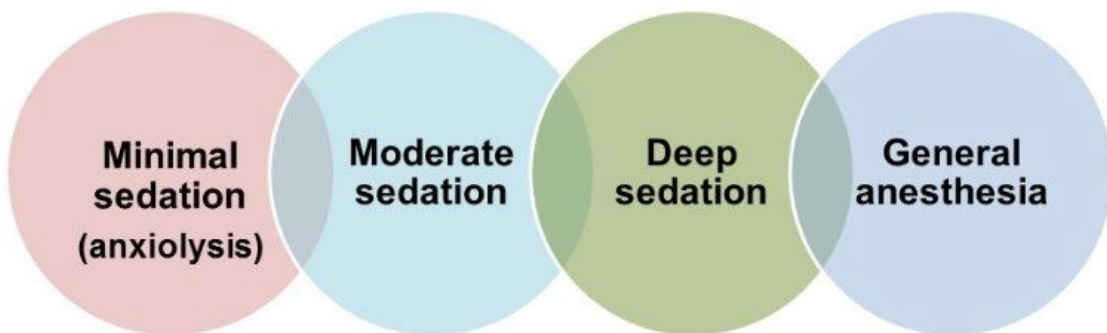

## Minimal Sedation

This is a continuum. To understand, we will begin with minimal sedation, also known as anxiolysis.

<b>Description</b>	<b>Minimal Sedation</b>	<b>Moderate Sedation/Analgesia</b>	<b>Deep Sedation/Analgesia</b>	<b>General Anesthesia</b>
<b>Responsiveness</b>	Normal response to verbal stimulation	Purposeful response to verbal or tactile stimulation	Purposeful response following repeated or painful stimulation	Unarousable even with painful stimulus
<b>Airway</b>	Unaffected	No intervention required	Intervention may be required	Intervention often required
<b>Spontaneous Ventilation</b>	Unaffected	Adequate	Maybe inadequate	Frequently inadequate
<b>Cardiovascular Function</b>	Unaffected	Usually maintained	Usually maintained	May be impaired

## Minimal Sedation (Anxiolysis)

### Key Points – Minimal Sedation

- Anxiolysis is medication therapy given to reduce anxiety and to help patients relax, e.g., diazepam (Valium) PO or midazolam (Versed) IVP prior to a procedure.
- The patient continues to respond normally to verbal commands.
- This level of sedation has no effect on airway, breathing, or the cardiovascular system.
- Cognitive function and physical coordination may be impaired.



## Moderate Sedation/Analgesia



<b>Description</b>	<b>Minimal Sedation</b>	<b>Moderate Sedation/Analgesia</b>	<b>Deep Sedation/Analgesia</b>	<b>General Anesthesia</b>
<b>Responsiveness</b>	Normal response to verbal stimulation	Purposeful response to verbal or tactile stimulation	Purposeful response following repeated or painful stimulation	No response even with painful stimulus
<b>Airway</b>	Unaffected	No intervention required	Intervention may be required	Intervention often required
<b>Spontaneous Ventilation</b>	Unaffected	Adequate	Maybe inadequate	Frequently inadequate
<b>Cardiovascular Function</b>	Unaffected	Usually maintained	Usually maintained	May be impaired

Page 7 of 21

## Moderate Sedation



During moderate sedation, the patient experiences a depressed level of consciousness during which they retain their ability to maintain a continuously patent airway. The patient will respond appropriately to physical stimulation and verbal commands, yet maintain partial amnesia.

The patient receives relief from anxiety and pain, allowing them to tolerate unpleasant procedures.

Moderate sedation/analgesia also expedites the course of procedures that are uncomfortable and require the patient to not move:

- Central line placements
- Scope procedures (endoscopy, bronchoscopy)
- Chest tube placement
- Painful wound debridements

Page 8 of 21

## Moderate Sedation *(cont.)*

### Key Points – Moderate Sedation

- The patient is able to respond to verbal commands.
- No interventions are needed to protect the airway or maintain heart rate and blood pressure, but close monitoring is essential.
- Cardiac monitoring is required for a patient with cardiovascular disease or dysrhythmia.
- Consents need to be signed before sedation is administered.



Page 9 of 21

## Clinical Characteristics of Moderate Sedation

Clinical characteristics of moderate sedation include:

- Maintenance of protective reflexes, i.e., gag reflex, ability to swallow, and ability to breathe without assistance.
- Independent and continuous maintenance of a patent airway.
- Purposeful response to physical stimulation and/or verbal commands.
- Easily aroused, with the provider talking in a normal tone of voice.
- Minimally depressed level of consciousness.
- Slightly slurred speech.

### Example:

In a normal tone of voice, the nurse asks the patient to take a deep breath and open their eyes. The patient should be able to follow this type of command at this level of sedation.

Page 10 of 21

## Clinical Characteristics of Moderate Sedation *(cont.)*

### Key Points – Moderate Sedation

- Important: A reflex withdrawal from a painful stimulus is not considered a purposeful response and is a sign the patient is progressing to general anesthesia.
- All practitioners involved with moderate sedation must be prepared to “rescue” the patient from a deeper level of sedation than was intended.



## Knowledge Check

During a procedure requiring moderate sedation, who is required to know how to rescue a patient from a deeper level of sedation than intended?

**(Choose all that apply.)**

- The registered cardiovascular invasive specialists (RCIS) assisting with the procedure
- The registered nurse (RN) assisting with the procedure
- The provider performing the procedure

## Deep Sedation/Analgesia

<b>Description</b>	<b>Minimal Sedation</b>	<b>Moderate Sedation/Analgesia</b>	<b>Deep Sedation/Analgesia</b>	<b>General Anesthesia</b>
<b>Responsiveness</b>	Normal response to verbal stimulation	Purposeful response to verbal or tactile stimulation	Purposeful response following repeated or painful stimulation	Unarousable even with painful stimulus
<b>Airway</b>	Unaffected	No intervention required	Intervention may be required	Intervention often required
<b>Spontaneous Ventilation</b>	Unaffected	Adequate	Maybe inadequate	Frequently inadequate
<b>Cardiovascular Function</b>	Unaffected	Usually maintained	Usually maintained	May be impaired

Page 13 of 21

## Deep Sedation

Deep sedation is used for procedures such as cardioversions, closed reductions of joint dislocations, or fractures. Patients who are deeply sedated cannot be easily aroused, but they do respond purposefully to repeated or painful stimulation, such as a vigorous sternal rub.

Page 14 of 21

## Deep Sedation *(cont.)*

**Key Point:** A reflex withdrawal from a painful stimulus is **not** considered a purposeful response and is a sign the patient is progressing to general anesthesia.



The patient's respiratory status may be affected and spontaneous respirations may be inadequate.

- Assistance may be needed to maintain a patent airway.
- Ventilation assistance may be required.

## Progression from Moderate to Deep Sedation

Clinical indications: Progression from moderate to deep sedation/anesthesia:

- Not easily aroused
- Partial or complete loss of protective reflexes
- Difficulty maintaining a patent airway independently
- Unable to respond to physical stimulation or verbal commands
- Severely slurred speech



**Key Point:**

**ALL practitioners involved with deep sedation MUST be prepared to “rescue” the patient from deep sedation or general anesthesia.**

## Progression from Moderate to Deep Sedation *(cont.)*

Clinical indications: Identifying a patient is in deep sedation:

- Similar to general anesthesia, the patient may be unable to maintain a patent airway.
- Loss of protective reflexes (unable to swallow, no cough, no gag reflex).
- The patient purposefully responds to repeated painful stimulation, such as a vigorous sternal rub.

	<i>Minimal Sedation Anxiolysis</i>	<i>Moderate Sedation/ Analgesia ("Conscious Sedation")</i>	<i>Deep Sedation/ Analgesia</i>	<i>General Anesthesia</i>
<i>Responsiveness</i>	Normal response to verbal stimulation	Purposeful** response to verbal or tactile stimulation	Purposeful** response following repeated or painful stimulation	Unarousable even with painful stimulus
<i>Airway</i>	Unaffected	No intervention required	Intervention may be required	Intervention often required
<i>Spontaneous Ventilation</i>	Unaffected	Adequate	May be inadequate	Frequently inadequate
<i>Cardiovascular Function</i>	Unaffected	Usually maintained	Usually maintained	May be impaired

## Knowledge Check



Characteristics of anxiolysis include: (Choose all that apply.)

- Reflex withdrawal from a painful physical stimulus
- Ability to respond normally to verbal commands
- Diminished respiratory rate or blood pressure
- Ability to maintain a patent airway
- Administering midazolam (Versed) to a stressed patient prior to a procedure

Page 19 of 21

## Knowledge Check *(cont.)*



Drag the type of sedation to the light blue box beside its description.

Type of Sedation	Description
Deep Sedation	The patient is unresponsive to verbal commands, but does purposefully respond to a sternal rub. Assistance may be needed to maintain a patent airway and adequate ventilation.
Minimal Sedation (Anxiolysis)	The patient continues to respond normally to verbal commands. This level of sedation has no effect on airway, breathing, or the cardiovascular system.
Moderate Sedation	The patient is able to open their eyes and raise their hand when asked.

Page 20 of 21

## References



American Society of Anesthesiologists. *Position on monitored anesthesia care*.  
Last amended on October 23, 2019.

Munson Healthcare Policies and Procedures. (2022, December 16). *Sedation*. PolicyStat.

# Procedural Sedation: Roles and Responsibilities

Amy Krug, BSN, RN, CGRN  
Lisa Lord, MSN, RN, CNOR  
Jeannette Reynolds, MSN, BBA, RN, CPAN

October 2023



## Goal and Objectives

### Goal

This course will ensure standardized practice for delivering sedation/analgesia during diagnostic and therapeutic procedures performed outside of the operating room, according to MHC policy. The ultimate outcome is to provide for the safety of our patients during sedation.

### Objectives

1. Identify who is qualified to order, administer, and monitor patients receiving moderate and deep sedation.
2. Describe the expected nursing care during procedural sedation.

Page 2 of 32



## Responsibilities

At MHC, Registered Nurses (RNs) and Registered Cardiovascular Invasive Specialists (RCIS) who will be monitoring sedated patients during procedures and administering moderate sedation are responsible for the following:

- Knowing the Sedation policy.
- Maintaining competence in sedation medication administration.
- Identifying when a patient has progressed to a deeper level of sedation than intended and intervening as needed.

**NOTE: RNs and RCIS do not administer deep sedation for procedures.**

Page 3 of 32

## Education Requirements

The education requirements for RNs and RCISs include:

Upon hire:

- Current BLS certification.
- Completion of the online HealthStream assignment.
- Completion of the airway station during RN orientation.
- Completion of the cardiac rhythm competency, the Basic ECG interpretation exam, or current ACLS certification.

Periodically thereafter:

Completion of periodic sedation education and demonstration of competence.

Page 4 of 32

## Provider Credential Check

MUNSON HEALTHCARE

Directories Help Desk my>HR News VOICE

Search this site

Tools & Resources Departments Education Human Resources

Give the gift of a blood donation. Click for more information.

At MHC, all physicians, physician assistants (PAs), nurse practitioners (NPs), and oral surgeons must be credentialed to provide sedation/analgesia.

Credential information is available via MHC Intranet.

**Click** Tools & Resources.

# Provider Credential Check



Search this site

At MHC, all physicians, physician assistants (PAs), nurse practitioners (NPs), and oral surgeons must be credentialed to provide sedation/analgesia.

Credential information is available via MHC Intranet.

Click Tools & Resources.

Click Physician Privileges.

Tools & Resources	Departments	Education	Human Resources
Change Management	Interpreter/Translation	SDS	
Directories	Library Services	System Documents	
Disaster Preparedness	Management Team Site		
Diversity, Equity, and Inclusion	Munson Healthcare Internet		
Downtime	MVP		
MHC Daily On Call Schedule	No Surprise Act		
Forms	Physician Privileges		
Hotel Workspace Bookings	PolicyStat		
ICD-10	Sepsis		

# Provider Credential Check



Search this site

At MHC, all physicians, physician assistants (PAs), nurse practitioners (NPs), and oral surgeons must be credentialed to provide sedation/analgesia.

Credential information is available via MHC Intranet.

Physician Services

CMO Corner

Payer Enrollment Status

**Provider Privileges**

Anesthesia Training

## Provider Privileges

Provider privileges at Munson Healthcare are available in the following searchable databases by facility.

Munson Medical Center (Traverse City):  
VerityStream/Morrisey MSOW database

Cadillac, Charlevoix, Grayling and Manistee Hospitals; Otsego Memorial Hospital (Gaylord); Paul Oliver Memorial Hospital (Frankfort); Kalkaska Memorial Health Center: MS SharePoint database — enter search criteria below.

Facility:  Provider Name:

## Knowledge Check

Who can administer moderate and deep sedation for procedural sedation (assuming they have the proper credentials and have completed the education)? (Choose all that apply.)

- Oral Surgeon
- ICU RN who is ACLS-certified
- Physician
- Physician Assistant
- Nurse Practitioner

## Pre-procedure Responsibilities: Provider Assessment

The proceduralist/provider is required to complete a comprehensive assessment of the patient prior to performing the procedure. This includes:

- A determination of the patient's American Society of Anesthesiologists Classification (ASA Class).
  - This is used as a guideline for **NPO status**.
- An airway assessment.



### **Key Points:**

- Anesthesiology can be consulted on any case, but consultation is **advisable** for patients with an **ASA Class of IV or V**. (See next page for description.)
- The pre-procedure assessment must be documented by the anesthesia provider.

## Pre-procedure Responsibilities: ASA Classification



American Society of Anesthesiologists Classification ("ASA Class") <sup>6</sup>	
ASA I	A normal healthy patient
ASA II	A patient with mild systemic disease
ASA III	A patient with severe systemic disease that limits activity but is not incapacitating
▶ ASA IV	A patient with severe systemic disease that is a constant threat to life
▶ ASA V	A moribund patient who is not expected to survive without the operation or procedure
ASA VI	A declared brain-dead patient whose organs are being removed for donor purposes

▶ = Anesthesia consultation advised.

## Pre-procedure Responsibilities: RN/RCIS Role



The RN or RCIS assisting with a procedure requiring sedation must ensure the following documentation is complete:

- Patient/family education
- Patient monitoring during procedure
- Time-based documentation during procedure

Prior to the procedure, the RN/RCIS must ensure all necessary supplies and equipment are available.



## Pre-procedure Responsibilities: Patient Preparation



Procedural sedation preparation is the same as any other procedure or surgery.

- Ensure all orders and diagnostic tests are complete, e.g., lab tests, x-rays, skin preps, etc.
- Verify the patient's NPO status. Follow orders based on ASA class.
- Educate the patient and family regarding the procedure scheduled and expectations of sedation; CONSENT SIGNED prior to any administration of sedation.

Page 10 of 32

## Pre-procedure Responsibilities: Patient Preparation *(cont.)*



Validate all required components are complete:

1. Valid H&P is less than 30-days old with reassessment of the patient documented within 24-hours of admission prior to the procedure.
2. Validation of the correct surgical/invasive procedure
3. Evaluation immediately prior to the procedure
4. Medications
5. Allergies and previous drug reactions
6. Patient's age
7. Patient's weight
8. Pre-procedure laboratory and other diagnostic testing
9. Consent

Page 11 of 32

## Pre-procedure Responsibilities: Patient Preparation (cont.)



- Ensure a comprehensive assessment of the patient is completed.
- Perform a baseline pain assessment.
- Verify patent IV access.
- Pre-oxygenate the patient via nasal cannula at a flow rate of 2 L/m (unless medically contraindicated).
- Verify emergency equipment is available and in working condition.
- Identify the patient, using two identifiers. Validate the correct patient, procedure, and site.
- Perform a time-out prior to beginning the procedure.



Page 12 of 32

## Pre-procedure Responsibilities: The Modified Aldrete Score (or validated tool)



Modified Aldrete Scoring is a measurement tool rating post-procedure recovery of consciousness, activity, respirations, and blood pressure.

- A pre-procedural Aldrete score is necessary to establish an accurate baseline of the patient's status.
- Pre-existing conditions should be considered when evaluating the patient's score.
- A post-procedural score should equal the pre-procedural baseline score prior to discharge from the recovery area.



**PRINT** the Modified Aldrete Scoring document **for use with answers on the quiz.**



Page 13 of 32

### Attachment A: Modified Aldrete Scoring by Age Group [Copy Link](#)

Adult Scoring Guideline Ages Greater than 12 Years		
Component	Scoring Guideline	Score
Activity	Voluntary & purposeful movement of extremities = 2 Non-voluntary or non-purposeful movement of extremities = 1 Unable to move extremities = 0	A
Respirations	Respirations even and non-labored = 2 Dyspnea or limited breathing = 1 Apnea = 0	B
Circulation	B/P within 20% of pre-procedure level = 2 B/P within 50% of pre-procedure level = 1 B/P < 50% of pre-procedure level = 0	C
Consciousness	Fully alert = 2 Arouses with name = 1 Unresponsive to pain = 0	D
Oxygen Saturation	≥ 92% on room air = 2 Needs O <sub>2</sub> to keep sat > 92% = 1	E

## Knowledge Check

The Modified Aldrete Scoring Guideline used to compare the patient's pre- and post-sedation status includes: (Choose all that apply.)

- Activity
- Respirations
- Pulse
- Cardiac rhythm
- Blood pressure

## Pre-procedure Responsibilities: Baseline Assessment



**Immediately prior** to medication administration, assess the following baseline parameters:

- Blood pressure
- Heart rate
- Respiratory rate
- Oxygen saturation
  - Maintain adult SpO<sub>2</sub> ≥ 92% and pediatric SpO<sub>2</sub> ≥ 95%.
- End-tidal CO<sub>2</sub> level
  - Maintain CO<sub>2</sub> at 35 – 45 mmHg.
  - The CO<sub>2</sub> level will increase if the patient's ventilatory status is compromised.
- Level of consciousness
- Cardiac rhythm
  - Continuous ECG monitoring is required for **all** patients with a cardiac history or expected dysrhythmias, and for **all** deep sedation cases.
- Modified Aldrete score

Page 16 of 32

## Knowledge Check



Pre-oxygenation at 2 L/m via nasal cannula is required for all procedural sedation cases, unless medically contraindicated.

- True
- False

Page 17 of 32

## Pre-procedure Responsibilities: Time-Out



Key Point: A “time-out” is **mandatory** prior to the start of the procedure.



During the time-out, the entire procedural team must pause, including the patient when possible, and verify the:

- Correct patient, using two patient identifiers
- Correct procedure
- Correct site (if applicable), including laterality

There must be **100% agreement** of the team **prior to starting** the procedure.

The time-out **must be documented** in the patient’s medical record.

## Intra-procedure Responsibilities: Monitoring



At a minimum, the following parameters should be monitored and documented **after every medication administration** and **every 5-10 minutes** during the procedure, following each additional dose of medication and more frequently as the patient’s clinical needs dictate.

- Blood pressure
- Heart rate
- Respiratory rate
- Oxygen saturation
  - Maintain adult SpO<sub>2</sub> ≥ 92%
  - Maintain pediatric SpO<sub>2</sub> ≥ 95%.
- Identification and management of adverse events
- Level of consciousness
- Medication: dose, route, time
- Modified Aldrete score
- Pain level
- EtCO<sub>2</sub> level

## Intra- & Post-procedure Assessment Considerations



Monitor the following to determine the patient's tolerance to the procedure:

- Significant variances in blood pressure, heart rate, respiratory rate and effort, SpO<sub>2</sub>, and end-tidal CO<sub>2</sub>.
- The patient's response or lack of response to verbal and physical stimuli.
- Facial grimacing and physical posturing, tensing, or flaccidity.

When observing the above, ask yourself:

- "Is the patient sedated enough?"
- "Is the patient experiencing pain?"
- "Is the patient over-sedated or at risk of being over-sedated?"

## Post-procedure Monitoring



Post-procedure, the following page lists parameters which should be monitored continuously and documented **every 15 minutes**, depending on the patient's condition and the procedure performed.

Documentation will continue through the post-procedure period until the patient reaches 8 or greater on the Modified Aldrete score.

## Post-procedure Responsibilities: Monitoring



At a minimum, the following parameters should be monitored and documented **after every medication administration** and **every 5-10 minutes** during the procedure, following each additional dose of medication and more frequently as the patient's clinical needs dictate.

- Blood pressure
- Heart rate
- Respiratory rate
- Oxygen saturation
  - Maintain adult SpO<sub>2</sub> ≥ 92%
  - Maintain pediatric SpO<sub>2</sub> ≥ 95%.
- Identification and management of adverse events
- Level of consciousness
- Medication: dose, route, time
- Modified Aldrete score
- Pain level
- EtCO<sub>2</sub> level

Page 22 of 32

## Post-procedure Responsibilities: Monitoring *(cont.)*



- Blood pressure
- Heart rate
- Respiratory rate
- Oxygen saturation
  - Maintain adult SpO<sub>2</sub> ≥ 92%
  - Maintain pediatric SpO<sub>2</sub> ≥ 95%.
- Identification and management of adverse events.
- End-tidal CO<sub>2</sub> level
  - Maintain CO<sub>2</sub> at 35 – 45 mmHg.
  - The CO<sub>2</sub> level will increase if the patient's ventilatory status is compromised.
- Cardiac rhythm
  - Continuous ECG monitoring is required for **all** patients with a cardiac history or expected dysrhythmias and for **all** deep sedation cases.
- Level of consciousness
- Medication: dose, route, time
- Modified Aldrete score
- Pain level
- Nausea

Page 23 of 32



## Post-procedure Assessment Considerations

- Patients may continue to be at significant risk for persistent/residual sedation effects or for developing complications after the procedure is completed.
- The reassessment and documentation of vital signs will revert to unit-specific standards of practice once the post-procedure monitoring criteria have been met.
- The patient's pain level may become more acute as the level of sedation decreases and will need to be treated accordingly.

Page 24 of 32




## Post-procedure and Over-Sedation

Over-sedated patients will require an extended recovery period.



### Key Points:

- Monitor Patient - If the patient received a reversal agent due to over-sedation, they must be monitored for a minimum of two hours after the last dose of the reversal agent.
- Submit a **VOICE** File:
  - When a reversal agent is used to rescue a patient.
  - If there are any complications or adverse outcomes.

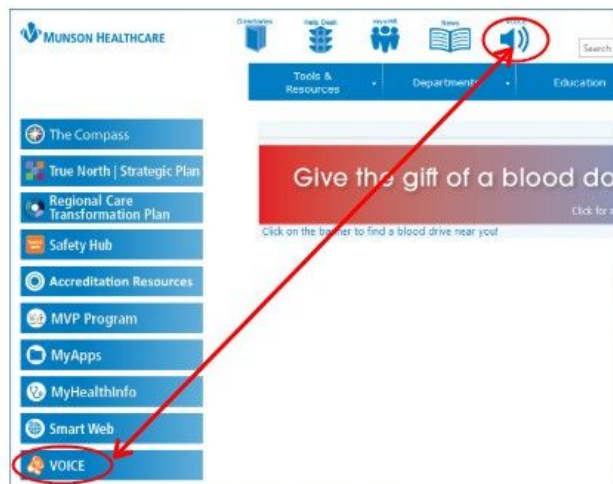

Page 25 of 32

## Discharge from Procedural Units

Patients are either discharged to their inpatient unit or discharged to home from the procedural unit.

Patients may be discharged when **at least** 30 minutes have elapsed since the last dose of sedation/analgesia was given.



### Key Points:

If a reversal agent was administered, the patient must be monitored for at least 2 hours after the last dose of reversal agent was given.

Monitoring can continue on an inpatient unit.

## Discharge Criteria

Prior to discharge, the following criteria must be met:

- Vital signs must be stable.
- Modified Aldrete score must be  $\geq 8$ .
- None, or mild nausea with no active emesis.
- Patient is arousable with protective reflexes intact.
- Pain-free, mild discomfort, or controlled with analgesics.
- Mobility must be back to pre-procedure baseline.

## Interpreting the Modified Aldrete Score

A patient requires either **a score  $\geq 8$**  or **a proceduralist/provider's order** to be transferred or discharged from the procedural unit. Other department/procedural-specific discharge criteria may also need to be applied.



### Key Point:

A score  $< 8$  indicates the patient should be closely monitored with interventions applied as indicated.

## Discharging Inpatients vs. Outpatients

### Inpatients:

- A full hand-off report must be given to the next provider of care.

### Outpatients:

- Written discharge instructions must be reviewed with the patient and responsible party.
- Discharge instructions include the hospital- and department-specific instructions and the 24-hour minimum restrictions mandated for patients who have received pain or sedative agents, including an emergency phone number.



### Key Point:

A responsible individual **must** be available to transport the patient home.



## Knowledge Check

You are caring for a patient immediately post-bronchoscopy. She is very groggy, but arouses when you call her name. She can move her extremities when asked, but she keeps falling back to sleep. Her respirations are non-labored, but her respiratory rate is 9-10. Her blood pressure is 108/68 (baseline was 124/78). She needs O<sub>2</sub> at 2 L/m via nasal cannula to keep her oxygen saturation at 93%.

What is her Modified Aldrete Score?

- 4
- 5
- 6
- 7
- 8

Page 30 of 32



## Knowledge Check *(cont.)*

Continuing with the same patient in the previous question, what does her score need to be for her to be discharged from the procedural area?

- Greater than or equal to 4
- Greater than or equal to 6
- Greater than or equal to 8
- Greater than or equal to 10

Page 31 of 32



## Reference

Munson Healthcare Policies and Procedures. (2022, December 16). *Sedation*.  
PolicyStat.

# Symptom Management for Procedural Sedation

Amy Krug, BSN, RN, CGRN  
Lisa Lord, MSN, RN, CNOR  
Jeannette Reynolds, MSN, BBA, RN, CPAN

October 2023

## Goal and Objectives

### Goal

This course will increase the participant's knowledge of managing potential symptoms associated with patients receiving procedural sedation.

### Objectives

1. Identify when a patient has progressed to a deeper level of sedation.
2. Identify nursing interventions appropriate to the patient's rescue needs.

## Common Side Effects of Sedation

The most common side effects of sedation administration are:

- Respiratory depression
- Hypotension
- Nausea and vomiting
- Paradoxical response

The most common adverse effect of opioids, especially when combined with sedatives, is respiratory depression.

If left untreated, respiratory depression can progress to apnea, followed by cardiac arrest.

EtCO<sub>2</sub> and pulse oximetry may show early signs of respiratory distress.



Page 3 of 17

## Treatment of Respiratory Depression

- **Stop all administration of opioids and sedatives!**
  - The duration of these medications depends on the drug, dose, route of administration, and the patient's condition.
- Maintain an open airway:
  1. Reposition the head/neck using the chin-lift or jaw-thrust.
  2. Provide oxygen therapy. Be prepared to use an ambu bag if necessary.
  3. Insert a nasal or oropharyngeal airway as necessary.
- If airway management is not effective, administer the appropriate reversal agent:
  - Flumazenil (Romazicon) for benzodiazepines.
  - Naloxone (Narcan) for opioids.
- Call MRT as appropriate.

**If the patient does not respond to airway management maneuvers and the reversal agent, call a Code Blue (5-5555)!**

Page 4 of 17



## Knowledge Check

The most common side effect of sedation administration is:

- Respiratory Depression
- Paradoxical Response
- Nausea and Vomiting
- Hypotension

Page 5 of 17



## Knowledge Check *(cont.)*

If respiratory depression occurs while I am assisting with a procedure that requires sedation, I should do all of the following: (Choose all that apply.)

- Reposition the head/neck by tucking the chin to the chest.
- Provide oxygen therapy, assisting with ventilation, if necessary.
- Insert an oropharyngeal airway, if needed.
- Administer the appropriate reversal agent.

Page 6 of 17

## Hypotension

Hypotension is most likely caused by vasodilation, blood loss during the procedure, or a pre-existing condition, but could also be caused by sedation.

The cause of the hypotension determines the treatment.

Possible treatments:

- IV fluid replacement
- Vasopressors
- Blood transfusion
- If you suspect the cause is over-sedation, administer reversal agents per protocol:
  - Flumazenil (Romazicon) for benzodiazepines.
  - Naloxone (Narcan) for opioids.




## Nausea and Vomiting

**Aspiration is a major concern with the patient receiving sedation.**

Treatment for nausea and vomiting:

- Position the patient to prevent aspiration. The preferred position is Semi-Fowlers with the head of the bed at 30 degrees and the patient on his/her side.
- Suction as necessary to maintain a patent airway.
- Administer an antiemetic.
- Patient to remain NPO until awake and alert.

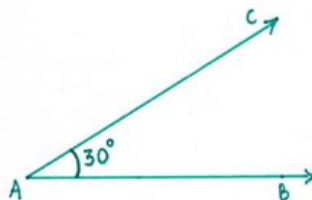



## Paradoxical Responses

The desired effect of moderate sedation or analgesia is a relaxed and cooperative patient. The patient is sedated but can be aroused and is able to follow simple commands.

If a patient has a sensitivity to a specific drug, a paradoxical response can occur. Consider a paradoxical response if the patient becomes any of these:

- Agitated
- Uncooperative
- Combative
- Disoriented



## Paradoxical Responses *(cont.)*

A thorough patient assessment is imperative to determine the actual cause of the patient's symptoms.

Paradoxical responses are seen more often in patients with a history of alcohol or IV drug abuse (most frequent).

Other causes to consider include:

- Hypoventilation due to hypoxia.
- Inadequate dosing of pain medication during a painful procedure.

## Over-sedation




### Symptoms:

- Decreased respiratory function (hypoventilation, decreased respiratory rate, or apnea)
- Decreased cardiovascular function (hypotension or dysrhythmias)
- Confusion
- Decreased level of consciousness that can progress to coma
- Depressed/absent cough and gag reflex
- Decreased response to physical/verbal stimuli

Page 11 of 17

## Treatment of Over Sedation



### Treatment:

- Ensure an open airway.
- Encourage or stimulate the patient to breathe.
- Administer supplemental oxygen to increase or maintain oxygen saturation greater than or equal to 92%.
- Ventilate with ambu bag if spontaneous ventilation is inadequate.
- Administer reversal agents per protocol:
  - flumazenil (Romazicon) for benzodiazepines.
  - naloxone (Narcan) for opioids or narcotics.
- If hypotensive, infuse IV fluids or consider vasopressors.
- Reposition patient to semi-fowlers.
- Consider MRT or RT evaluation, if appropriate.
- If patient uses home CPAP/BiPAP, also use it post-procedure.

**If the patient does not respond to airway management maneuvers and the reversal agent, call a Code Blue (5-5555)!**

Page 12 of 17



## Knowledge Check

Symptoms of over-sedation include: (Choose all that apply.)

- Decreased response to stimuli
- Decreased respiratory rate
- Agitation
- Hypotension

Page 13 of 17



## Knowledge Check *(cont.)*

If a patient is in respiratory arrest and does not respond to airway management and reversal agents, I should:

- Call a Code Blue.
- Call and MRT.
- Call the provider.

Page 14 of 17

## Reporting Requirements

**Whenever it is necessary to administer a reversal agent, a VOICE file must be completed. Access the form from the MHC Intranet.**

Other complications related to sedation to be reported include:

- Incidents in which the patient slips into a level of sedation that is greater than intended, e.g., moderate to deep sedation.
- Profound hypotension (50% decrease from pre-procedure mean blood pressure)
- Cardiac arrest
- Defibrillation
- Respiratory arrest
- Seizures
- Aspiration
- Medication errors
- Vomiting



## Knowledge Check

I must fill out a VOICE file for the following situations: (Choose all that apply.)

- If a patient slips into a deeper level of sedation than intended.
- Profound hypotension
- Medication errors
- If a reversal agent is required to control an adverse reaction, such as respiratory depression.



## References

- Munson Healthcare Policies and Procedures. (2022, December 16). *Sedation*. PolicyStat.
- Munson Healthcare Policies and Procedures. (2021, April 20). *Flumazenil Protocol*. PolicyStat.
- Munson Healthcare Policies and Procedures. (2022, February 21). *Standing Order/Protocol for Adult Naloxone (Narcan)*. PolicyStat

# Procedural Sedation Medication Guidelines

Lauren Wolf, PharmD, BCPS, BCCCP

December 2025

## Goal and Objectives



### Goal

This course will increase the participant's knowledge of administering medications for procedural sedation.

### Objectives

1. Identify staff who can administer sedation.
2. Select the appropriate medication and dose for reversing over sedation.

## Introduction

Dosage guidelines for procedural sedation and reversal agents are approved by the Pharmacy and Therapeutics (P & T) Committee at Munson Medical Center.

These guidelines are intended for initial doses and may be exceeded or decreased according to the patient's history, previous response to sedatives or other clinical circumstances.

Prior to administration, the P & T Committee must review and approve the use of all medications not listed in the approved guidelines.



Page 3 of 30

## Guidelines Location

Nurses and Registered Cardiovascular Invasive Specialists (RCIS) should be familiar with medication guidelines before administering sedation. The medication guidelines are attached to the Sedation policy.

Moderate & Deep Sedation/Analgesia Drug Usage Guidelines are listed below. [Print](#) the document to use as a reference for upcoming questions.

Attachment C: Moderate Sedation/Analgesia Drug Usage Guidelines

A. IVP by RN or ED Trained Pharmacist in the presence of the provider credentialed for moderate sedation

B. Not intended for Neonates - Unless otherwise indicated

Drug	Pharmacokinetics	Drug Dosage & Administration	Precautions / Contraindications
Diazepam (Valium)	<u>Onset:</u> IV: 1-3 min	<u>Adults IV:</u> 5-10mg - no faster	<ul style="list-style-type: none"><li>Titrate to effect. Do not dilute.</li></ul>

## Facility-specific IV Push and Infusion Guidelines



Munson Healthcare has an IV Push/Infusion Chart to assist staff with decisions regarding the administration of medications. This chart can be found on the Intranet on the Pharmacy Department site.

The chart contains various topics, including:

- Medications administered by IV push or by infusion.
- Approved medications per department.
- Medications a nurse can give during a Code Blue.
- Medications requiring a physician be present during administration.

**NOTE:** See the IV Push Chart on the next slide.

Page 5 of 30

## MMC IV Push Chart



Navigation bar with icons for back, forward, search, and other controls.

### MUNSON HEALTHCARE IV MEDICATION ADMINISTRATION GUIDELINES

#### Definitions

<b>Level 1</b>	Units with general nursing and monitoring capabilities (ex. med-surg).
<b>Level 2</b>	Intermediate and telemetry units. RNs working on these units have more advanced training and advanced monitoring (telemetry) are present. Level 2 may be further divided into level 2a (telemetry units) or level 2b (step-down units)
<b>Level 3</b>	Critical and emergency care units (including operating rooms). Licensed clinicians working on these units are trained to manage emergencies and manage critically ill patients. Advanced monitoring and treatment resources are readily available.
<b>OB</b>	Birth units and units dedicated to the care of antepartum and postpartum patients. OB units follow level 1 criteria noted.
<b>PEDS</b>	Any unit caring for patients 18 years of age or less. Peds may be further subdivided as <b>level 1, level 2, and level 3</b> criteria above.

#### Exclusions

- Chemotherapy/antineoplastic agents
- Biologics and immune therapies typically restricted to outpatient administration (ex. Infliximab, vedolizumab)
- Basic IV hydration fluids (ex. 0.9% normal saline, Normosol, lactated ringers)
- Non-intravenous parenterally administered medications

## Who Can Administer Sedation?



Medications for **moderate** sedation may be given by a registered nurse (RN) or registered cardiovascular invasive specialist (RCIS) in the presence of the physician, physician assistant (PA), nurse practitioner (NP), or oral surgeon credentialed in moderate sedation and in advanced airway management.

## Who Can Administer Sedation? *(cont.)*



Medications for **deep** sedation, can **ONLY** be administered by a provider credentialed in deep sedation.

➤ **Exception: Propofol** - a critical care RN may give propofol (Diprivan) IVP for an emergent intubation while a physician is present and performing the intubation.

- Critical care is defined by the IV Push/Infusion Chart to include these units:
  - ✓ ICU
  - ✓ ED
  - ✓ PACU
  - ✓ OR
  - ✓ A2 (critical)
  - ✓ A3 (critical)
  - ✓ IR



## Knowledge Check

A patient is scheduled for a wound debridement at the bedside. The physician orders hydromorphone (Dilaudid) 0.1-0.5mg IV titrated over 1 minute for moderate sedation.

This is an approved dose according to the MMC Moderate Sedation Guidelines.

- True
- False

Page 9 of 30



## Knowledge Check *(cont.)*

A patient is scheduled for a synchronized cardioversion. The physician orders propofol (Diprivan) at 1mg/kg per minute over 60 seconds.

How long do the effects of propofol (Diprivan) last?

- 1-2 minutes
- 3-10 minutes
- 12-20 minutes
- 25-30 minutes

Page 10 of 30



## Knowledge Check *(cont.)*

A registered nurse from the ICU can give propofol (Diprivan) IV push with a physician order, if the physician is present in the room, but is not intubating the patient.

- True
- False

Page 11 of 30



## Reversal Agents

- Reversal agents may be indicated when:
  - The level of sedation is deeper than desired.
  - The patient's responsiveness or cardio-respiratory status is compromised.
  - An idiosyncratic reaction occurs.
- If a reversal agent is administered for the undesired effects, a **VOICE** file is required.
- A patient should be monitored for a minimum of two hours after giving a reversal agent.

Page 12 of 30



## Commonly Used Opioids

If a patient becomes difficult to arouse with verbal or physical stimuli related to sedation from an opioid, follow the Standing Order/Protocol for Adult Naloxone (Narcan) Protocol. The naloxone (Narcan) protocol can be located:

- Policy website on the Intranet
- Pharmacy website on the Intranet
- Side of the crash cart

Examples of commonly used opioids include:

Codeine	Morphine
Demerol (meperidine)	Norco (hydrocodone + acetaminophen)
Dilaudid (hydromorphone)	Oxycontin (oxycodone)
Dolophine (methadone)	Percocet (oxycodone + acetaminophen)
Duragesic (fentanyl patch)	Sublimaze (fentanyl injection)



## naloxone (Narcan) Protocol

The naloxone protocol allows the registered nurse or RCIS to:

- Titrate oxygen to maintain an oxygen saturation of at least 92%.
- Perform further interventions, including the administration of naloxone depending on the patient's mental status and O<sub>2</sub> saturation.
- For patients with oxygen saturations  $\geq$  to 80%, dilute the naloxone 0.4 mg in 9 ml of normal saline and administer in small, 1mL doses following the protocol. This allows for better titration of the dosing [so the patient doesn't over respond to the naloxone and end up in severe pain].
- Give naloxone 0.4 mg **undiluted** for an O<sub>2</sub> saturation below 80% or respiratory arrest.

**NOTE:** Click the button.

Review the naloxone  
(Narcan) Protocol



Show Changes

Tag Policy

## Standing Order/Protocol for Adult Naloxone (Narcan)

### Purpose

To provide a policy for Adult Naloxone (Narcan) standing orders/protocols.

### Policy

A. The Protocol for Adult Naloxone (Narcan) shown below, is approved as a standing order and may be initiated by a Registered Nurse (RN) or Licensed Practical Nurse (LPN) without a provider order for any patient if:

1. Patient is difficult to arouse with verbal/physical stimuli ~AND~
2. Patient is on, or recently was on, opioids or suspected that the patient has consumed opioids



. This protocol is not applicable for end of life/palliative or comfort care/hospice patients. Call provider to clarify if any questions.

C. If criteria above are met then the initiating provider will enter by Physician Order Entry (POE) using

Page 16 of 30



## naloxone (Narcan) Points to Remember

- The onset of action for naloxone is within 2 minutes.
- The half-life of naloxone is 30-90 minutes.
- Many opioids have a longer half-life than naloxone, so it is important to monitor your patients closely. A repeat dose of naloxone may be required.



## Knowledge Check

A 52-year-old female was admitted post-intervention to her right coronary artery. She received an initial dose of morphine sulfate 2 mg IV push prior to her sheath pull. She continued to complain of discomfort @ 8/10. An additional morphine sulfate 4 mg IV push was administered for discomfort. Respirations are now 5/minute; oxygen saturation is 82%. The patient is not arousable to verbal stimuli, but is arousable to a sternal rub.

Which dose of reversal agent should be initiated?

- naloxone 0.4 mg diluted in 9 mL of normal saline, and give 1 mL IV push
- naloxone 0.4 mg diluted in 9 mL of normal saline, and give IV push
- naloxone 0.4 mg IV push (undiluted)
- naloxone 0.4 mg diluted in 9 mL of normal saline, and give 2 mL IV push



## Treating Over Sedation from a Benzodiazepine

If a patient becomes difficult to arouse with verbal or physical stimuli related to sedation from a benzodiazepine, follow the flumazenil (Romazicon) protocol.

The flumazenil protocol can be located:

- Policy website on Intranet
- Pharmacy website on Intranet
- Side of the crash cart

## Commonly Used Benzodiazepines

The most commonly used benzodiazepines are:

<b>alprazolam (Xanax )</b> ★	flurazepam (Dalmane)
chlordiazepoxide (Librium)	<b>lorazepam (Ativan)</b> ★
clonazepam (Klonopin)	<b>midazolam (Versed)</b> ★
clorazepate (Tranxene)	oxazepam (Serax)
<b>diazepam (Valium )</b> ★	<b>temazepam (Restoril)</b> ★
estazolam (Prosom)	triazolam (Halcion)

★ = MMC formulary benzodiazepines

## flumazenil (Romazicon) Protocol

The flumazenil Protocol allows the registered nurse or RCIS to:

- Titrate oxygen to maintain an oxygen saturation of at least 92%.
- Perform interventions, including administering flumazenil if the patient is unarousable AND:
  - Oxygen saturation is less than 89% **OR**
  - Respiratory rate is less than 6.
- Initial dose: flumazenil 0.2 mg IV push over 30 seconds

**NOTE:** Click the button to review the flumazenil protocol;  
check for repeat dosing and the complete intervention sequence.

Review the flumazenil  
(Romazicon) Protocol



Show Changes

manifest, POMH)  
Tag Policy

## Flumazenil Protocol

### Purpose


Flumazenil (Romazicon) protocol for suspected Benzodiazepine overdose in adults.

### Policy

#### Flumazenil Reversal Protocol (Physician Order Required)

**Purpose:** Flumazenil (Romazicon) protocol for suspected Benzodiazepine Overdose in Adults

- Most Common Benzodiazepines**
- Alprazolam (Xanax)
  - Chlordiazepoxide (Librium)
  - Clonazepam (Klonopin)
  - Clorazepate (Tranxene)
  - Diazepam (Valium)
  - Estazolam (ProSom)

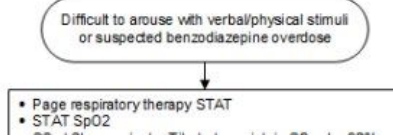

## flumazenil (Romazicon) Points to Remember

- The onset of action is 1-2 minutes.
- Duration:
  - Re-sedation occurs after approximately 1 hour (range: 19-50 minutes).
- Many benzodiazepines have a longer half-life than flumazenil, so it is important to monitor your patients closely. A repeat dose may be required.
- Avoid use of flumazenil in patients with chronic benzodiazepine use. Its use may precipitate seizures.



## Knowledge Check

You are assigned to an 88-year-old man who arose from a sitting position and had a syncopal episode. He was placed on the stroke unit for telemetry monitoring. At the start of your evening shift, he becomes very agitated. An order is obtained to give him lorazepam (Ativan). He finally falls asleep after 0300. At the end of the shift (0700), you find him difficult to arouse to both verbal and physical stimuli. His respirations are 5/minute and his oxygen saturation is 86%.

Which reversal dosing agent is appropriate for this patient?

- Undiluted naloxone (Narcan) 0.4 mg IV push STAT
- Diluted naloxone (Narcan) 0.4 mg in 9 mL normal saline
- flumazenil (Romazicon) 0.2 mg IV push over 30 seconds
- flumazenil (Romazicon) 0.4 mg IV push over 30 seconds

Page 23 of 30



## Selecting naloxone (Narcan) vs. flumazenil (Romazicon)

When a patient has received/taken both a benzodiazepine and an opioid, and a reversal agent is needed, **give the naloxone first.**

Reasons:

- Opioids are more likely to cause respiratory depression and other adverse effects, such as hypotension.
- flumazenil can cause seizures in patients with a history of long-term use of benzodiazepines.

Page 24 of 30



## Knowledge Check

A 21-year-old female patient has returned following endoscopy in the Medical Procedure Room. She received Demerol 75 mg and Versed 7.5 mg during the procedure.

She has a history of taking Xanax 0.25 mg three times per day for anxiety and Vicodin PRN for pain. She was discharged to B2 following an uneventful recovery with an Aldrete score of 8. Respirations are now 5/minute with an oxygen saturation of 85%. The patient is not arousable to verbal stimuli, but does arouse to a sternal rub.

Which reversal agent protocol should be used first?

- naloxone (Narcan) Protocol
- flumazenil (Romazicon) Protocol



## Knowledge Check *(cont.)*

A 21-year-old female patient has returned following endoscopy in the Medical Procedure Room. She received Demerol 75 mg and Versed 7.5 mg during the procedure.

She has a history of taking Xanax 0.25 mg three times per day for anxiety and Vicodin PRN for pain. She was discharged to B2 following an uneventful recovery with an Aldrete score of 8. Respirations are now 5 minute with an oxygen saturation of 85%. The patient is not arousable to verbal stimuli, but does arouse to a sternal rub.

Which dose of Narcan (naloxone) should be administered?

- naloxone 0.4 mg IV push (undiluted)
- naloxone 0.4 mg diluted in 9 mL of normal saline, and give IV push
- naloxone 0.4 mg diluted in 9 mL of normal saline, and give 2 mL IV push
- naloxone 0.4 mg diluted in 9 mL of normal saline, and give 1 mL IV push



## Treating Patients Who Revert to a Deeper Level of Sedation

- Remember, the effects of opioids and benzodiazepines last longer than the effects of the reversal agents.
- Continue to monitor the patient for signs of progression to a deeper level of sedation for a minimum of 2 hours.
- Repeated dosing of the reversal agents may be needed.
- Create and submit a **VOICE** file.

Page 27 of 30



## Dissociative Sedation

Dissociative sedation is a trance state where the patient remains awake, but is unaware of pain and will have no memory of the event.

- In comparison to deep sedation, which causes the patient to:
  - Be unarousable, except with repeated or painful stimuli
  - Experience respiratory depression

Page 28 of 30



## Ketamine for Dissociative Sedation

Ketamine will be administered by providers credentialed for deep sedation.

1. A pharmacist, nurse, or non-credentialed provider may administer medications for dissociative sedation in the Emergency Department, as long as a provider credentialed for deep sedation, an RN, and a respiratory therapist are **ALL** present.
2. Respiratory adverse events, such as apnea or laryngospasm (although uncommon), may still occur, and **providers must always be prepared to rescue the patient from a deep sedation state** anytime ketamine is administered.
3. Ketamine (IM/IV) is used for dissociative sedation in both children and adults (including the mentally disabled) for medical procedures such as, but not limited to: fracture reduction, laceration repair, abscess drainage, foreign body removal.
4. If Ketamine is administered IM, IV access should be immediately available.



## References

- Lexicomp. (2023, November 29). *Flumazenil*. Retrieved December 5, 2023.
- Munson Healthcare Policies and Procedures. (2021, April 20). *Flumazenil Protocol*. PolicyStat.
- Munson Healthcare Policies and Procedures. (2022, February 21). *Standing Order/Protocol for Adult naloxone (Narcan)*. PolicyStat.
- Munson Medical Center. (2023, October). *IV push/infusion chart - adult*.
- Munson Medical Center Policies and Procedures. (2022, December 16). *Sedation*. PolicyStat.



# Transducer system setup (MUNSON)



## Transducer system setup (MUNSON)

### ■ Introduction

The exact type of transducer system used depends on the patient's needs and the doctor's preference. Some systems monitor pressure continuously, others monitor pressure intermittently. Single-pressure transducers monitor only one type of pressure—for example, pulmonary artery pressure (PAP). Multiple-pressure transducers can monitor two or more types of pressure, such as PAP and central venous pressure.

### ■ Equipment

- Bag of flush solution (usually 500 mL normal saline solution)
- Pressure infusion bag
- Medication-added label
- Preassembled disposable pressure tubing with flush device and disposable transducer
- Monitor and monitor cable
- IV pole with transducer mount
- Leveling device
- Sterile, nonvented stopcock caps
- Sterile gauze package
- Optional: 500 to 1,000 units of heparin to add to flush bag

### ■ Implementation

To set up and zero a single-pressure transducer system, perform the following steps.

#### Setting up the system

- Gather the appropriate equipment.
- Perform hand hygiene.
- Put the pressure module into the monitor and connect the transducer cable to the monitor.
- Remove the preassembled pressure tubing from the package and tighten all tubing connections.
- Position all stopcocks to allow the flush solution to flow through the entire system.
- Roll the tubing's flow regulator to the OFF position.
- Spike the flush solution bag with the tubing, invert the bag, open the roller clamp, squeeze all the air from the drip chamber and compress the drip chamber.
- Place the flush solution bag into the pressure infuser bag.
- Open the tubing's flow regulator and prime the system, allowing no air to enter the system.

- Replace the vented caps on the stopcocks with sterile nonvented caps.
- Replace the protective cap at the end of the tubing after completely priming the system.
- Inflate the pressure infuser bag to 300 mm Hg.
- Perform hand hygiene.




- When the solution nears a stopcock, open the stopcock to air, allowing the solution to flow into the stopcock, as shown. When the stopcock fills, close it to air and turn it open to the remainder of the tubing. Do this for each stopcock.



- **Zeroing the system**

- Perform hand hygiene.
- Ask the patient to lie flat on the bed, if he can tolerate this position.
- Use a level to position the air-reference stopcock or the air-fluid interface of the transducer level with the phlebostatic axis.
- Turn the stopcock next to the transducer off to the patient and open to air.
- Remove the cap to the stopcock port and place it in an opened sterile gauze package.
- Zero the transducer by pressing the zero button on the pressure module or on the touch zero on Philips monitor screen.
- After zeroing, turn the stopcock on the transducer so that it's closed to air and open to the patient. Replace the cap on the stopcock.
- Perform hand hygiene.

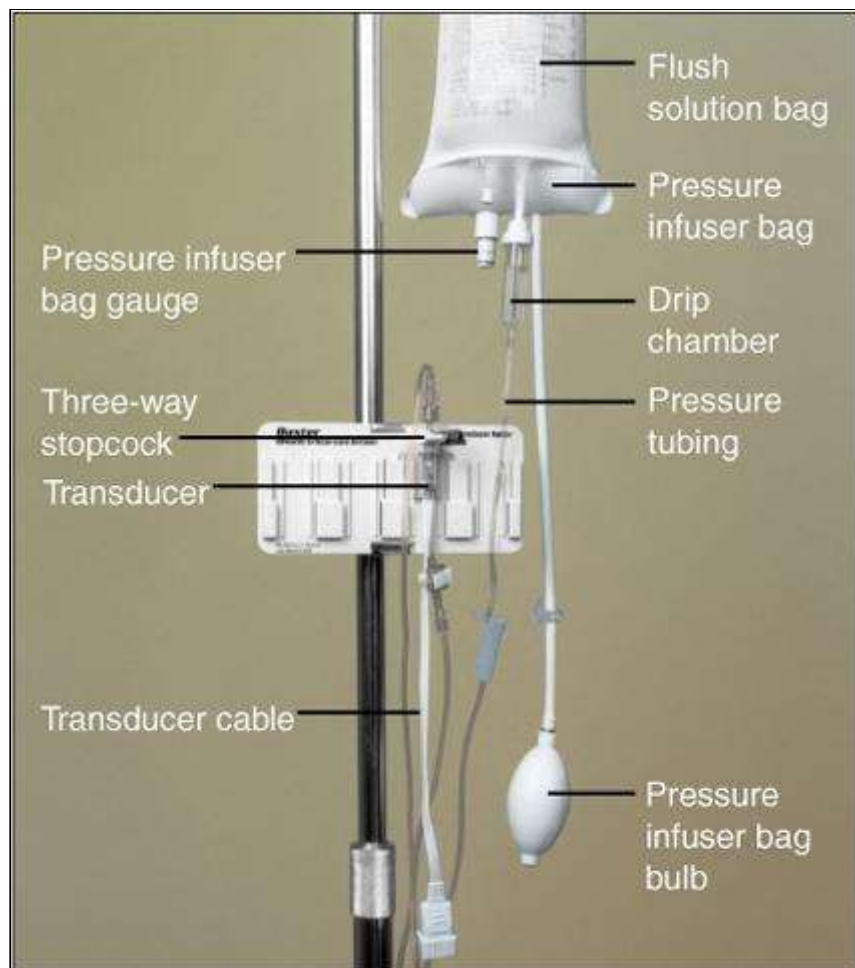

## ■ Special Considerations

- You may use any of several methods to set up a multiple-pressure transducer system. But the easiest way is to add to the single-pressure system. You'll also need another bag of heparin flush solution in a second pressure infuser bag. Then you'll prime the tubing, mount the second transducer, and connect an additional cable to the monitor. Finally, you'll zero the second transducer.
- Alternatively, your facility may use a Y-type tubing setup with two attached pressure transducers. This method requires only one bag of flush solution. To set up the system, proceed as you would for a single transducer, with this exception: First, prime one branch of the Y-type tubing and then the other. Next, attach two cables to the monitor in the modules for each pressure that you'll be measuring. Finally, zero each transducer.
- Minimize the number of manipulations and entries into the pressure monitoring system *to reduce the risk of infection.*<sup>[2]</sup>
- If the pressure monitoring system is accessed through a diaphragm instead of a stopcock, thoroughly disinfect the diaphragm with an antiseptic pad using friction before accessing the system.<sup>[2]</sup>
- Change the flush bag, tubing, and other components of the system every 96 hours, immediately when contamination is suspected or when the integrity of the product or system is compromised, or according to your facility's policy.<sup>[8]</sup> <sup>[2]</sup>

## ■ Documentation

Document the patient's position for zeroing so that other health care team members can replicate the placement. Document the flush solution used and the date and time of tubing changes.

## ■ References

[\(Rating System for the Hierarchy of Evidence for Intervention/Treatment Questions\)](#)

1. The Joint Commission. *Comprehensive Accreditation Manual for Hospitals: The Official Handbook*. Standard NPSG.07.01.01. Oakbrook Terrace, Ill.: The Joint Commission, 2011. (Level I)
2. Centers for Disease Control and Prevention. "Guideline for Hand Hygiene in Health-Care Settings," *Morbidity and Mortality Weekly Report* 51 (RR-16): 1-45, October 2002. (Level I)
3. World Health Organization. (2009). "WHO Guidelines on Hand Hygiene in Health Care: First Global Patient Safety Challenge, Clean Care is Safer Care." Geneva: World Health Organization. [Online]. Accessed April 2011 via the Web at [http://whqlibdoc.who.int/publications/2009/9789241597906\\_eng.pdf](http://whqlibdoc.who.int/publications/2009/9789241597906_eng.pdf). (Level I)
4. American Association of Critical Care Nurses. "Evaluation of the Effects of Heparinized and Nonheparinized Flush Solution on the Patency of Arterial Pressure Monitoring Lines: The AACN Thunder Project," *American Journal of Critical Care* 2(1):3-15, January 1993. (Level II)
5. Lalive, J.L. "Pulmonary Artery Pressure and Position Changes in the Critically Ill Adult," *Dimensions in Critical Care Nursing* 1(1):28-34, January-February 1982. (Level VI)
6. Lynn-McHale Wiegand, D., ed. *AACN Procedure Manual for Critical Care*, 6th ed. Philadelphia: Saunders, 2011.
7. Centers for Disease Control and Prevention. (2002). "Guidelines for the Prevention of Intravascular Catheter-Related Infections." Atlanta: Centers for Disease Control and Prevention. [Online]. Accessed April 2011 via the Web at <http://www.cdc.gov/hicpac/pdf/guidelines/bsi-guidelines-2011.pdf>. (Level I)
8. "Infusion Nursing Standards of Practice Standard 43: Administration Set Change," *Journal of Infusion Nursing* 34(1S):S55-57, January-February 2011. (Level I)

## ■ Notes

Des not apply at KMHC & POMH

### Rating System for the Hierarchy of Evidence for Intervention/Treatment Questions

The following leveling system is adapted from *Evidence-Based practice in nursing & healthcare: A guide to best practice*, Fifth edition, by Bernadette Mazurek Melnyk and Ellen Fineout-Overholt (2023).

<b>Level I</b>	Evidence from a systematic review or meta-analysis of all relevant randomized controlled trials (RCTs)
<b>Level II</b>	Evidence from well-designed single RCTs (experimental)
<b>Level III</b>	Evidence from well-designed nonrandomized controlled trials (quasi-experimental), systematic reviews of a complete body of evidence, and intervention studies using mixed methods
<b>Level IV</b>	Evidence from well-designed case-control and cohort studies (observational)
<b>Level V</b>	Evidence from systematic reviews of qualitative and descriptive studies
<b>Level VI</b>	Evidence from single descriptive and qualitative studies, evidence-based practice implementation, and quality improvement projects

**Level VII**

Evidence from expert opinion, expert committee reports, and literature reviews

*Data from Gyatt, G., & Rennie D. (2002). Users' guides to the medical literature. American Medical Association; Harris, R. P., et al. (2001). Current methods of the U.S. Preventative Services Task Force: A review of the process. American Journal of Preventative Medicine, 20, 21-35.*



Origination 2/14/2019  
Last Approved 8/14/2024  
Effective 8/14/2024  
Last Revised 8/14/2024  
Next Review 8/14/2027

Owner Joseph Santangelo: Chief Medical Quality & Safety Officer  
Area/Department Medical Staff  
Applicability Munson Healthcare Systemwide  
Tags Policy

# Universal Protocol: For Surgical and Non-Surgical Invasive Procedures

## Purpose

To provide a policy for surgical and non-surgical invasive procedures.

## Policy

- A. The Universal Protocol is a multi-disciplinary process encompassing the multiple phases of pre-surgical/procedural preparation to improve patient safety and prevent procedural errors.
- B. The Universal Protocol consists of three components, a pre-procedure verification process, marking of the surgical/procedural site and the time out just before starting the procedure.
- C. The protocol applies to all surgical and non-surgical invasive procedures. These procedures may occur in settings other than the Operating Room (OR), i.e. medical procedure room (MPR), emergency department (ED), radiology, cardiac diagnostic unit, nursing units, or ambulatory setting. Invasive procedures are procedures involving a puncture or incision to the skin, insertion of an instrument, or insertion of foreign material into the body. PICC lines, central line insertions, chest tube insertion, and other similar procedures are within the scope of the protocol.
- D. Refer to Addendum A for invasive procedures specific to the protocol. Minimal risk procedures such as venipuncture, peripheral line placement, NG tube insertions, or urinary bladder catheters are not part of the protocol.

# Pre-Procedure Verification Process

## A. Purpose

1. To ensure that all of the relevant documents, related information and/or equipment are:
  - a. Available prior to the start of the procedure
  - b. Have been correctly identified, labeled, and matched to the patient's identifiers
  - c. Have been reviewed and are consistent with the patient's expectations and with the team's understanding of the intended patient, procedure, and site. The patient (or guardian if the patient is a minor or incompetent) is involved in the verification process when possible.

## B. Process

1. An ongoing process of information gathering and verification, beginning with the decision to perform a procedure, continuing through all settings and interventions involved in the pre-procedure preparation of the patient, up to and including the "time out" just before starting the procedure. Missing information or discrepancies are addressed before starting the procedure. Pre-procedure verification is required for elective and emergent cases.

## Detailed Requirements

### A. Verification of the correct person, procedure, and site occurs:

1. At the time the procedure is scheduled.
2. At the time of preadmission testing and assessment.
3. At the time of admission or entry into the facility for a procedure whether elective or emergent.
4. Before the patient leaves the pre-procedure area or enters the procedure room.
5. Anytime the responsibility of care is transferred to another member of the procedural care team, (including the anesthesia providers) at the time of and during the procedure.

### B. Verification of the correct person, procedure, and site should occur as the final step in preparing the patient for an invasive procedure, prior to when the time-out occurs. When possible, the patient (or guardian if the patient is a minor or incompetent) should be involved in the process. Each department will determine the location where the verification process will occur (i.e., prior to the patient leaving the pre-procedure area or entering the procedure room).

### C. A standardized list will be used in the verification process to validate the correct patient, procedure, and site and to ensure all relevant items are available for the procedure.

1. At minimum, the list must include:
  - a. Patient identified using 2 patient identifiers
  - b. Validation of the correct procedure(s)

- c. Validation of the correct site(s)
  - d. Validation of the physicians order(s)
  - e. A valid consent form(s) that has been signed by the patient (or guardian if the patient is a minor or incompetent) and witnessed.
  - f. Relevant documentation, (i.e. a valid, relevant, updated H&P, consultation, or handwritten progress notes; nursing and pre-anesthesia/sedation assessment).
  - g. Correct diagnostic and radiology test results that are properly labeled, if applicable.
  - h. Required blood products, implants, devices, and/or special equipment available prior to start of the procedure, if applicable.
2. Each area may add additional items to the list, as applicable.
  3. Each area will be responsible to ensure the list is available and consistently used as a reference during the verification process.
  4. It is not necessary to document that a standardized list was used for each patient.

## Marking the Operative/Procedure Site

- A. For patient safety, regulations require uniformity in site marking practices to prevent errors. The method of marking the site and the type of mark is to be unambiguous and be used consistently throughout the organization. **The approved site marking is the initials of the person performing the procedure.**
  1. ***The person performing the procedure must do the site marking, this cannot be delegated. This individual must be directly involved and present at the time the procedure is performed.***
  2. Marking should take place with the patient involved, awake and aware, if possible.
  3. The mark is made at or near the procedure or the incision site. Do **NOT** mark any non-procedure site(s) unless necessary for some other aspect of care.
    - a. The mark must be visible after the patient's skin is prepped, the patient is in their final position and sterile draping is completed.
    - b. The mark must be made using a marker that is sufficiently permanent to remain visible after completion of the skin prep and sterile draping. Adhesive site markers are not used as the sole means of marking the site.
    - c. The procedural physician may elect to write certain aspects of the procedure with the site marking, such as the vertebral level.?
  4. Site marking is required for the following procedures involving incisions or percutaneous puncture or insertion of foreign material into the body.
    - a. Marking includes laterality, surface (flexor, extensor), the level (spine), specific lesion or digit to be treated.
    - b. For midline incision approach for organs of laterality, the site is still

- marked and the laterality noted.
- c. A wrist/ankle band labeled "Operative or Procedural Side" (written with an indelible marker) will be placed on the limb of the correct side for identifying laterality for a natural orifice or perineum approach.?
  - d. Spinal procedures require a two stage marking process, marking of the site and identification of the vertebral level(s).
    - i. Marking of the skin at the general spinal region.
    - ii. The use of radiographic intraoperative techniques is required to mark the exact vertebral level.
  - e. Interventional radiology cases where the side or individual structure is identified by imaging guidance during the procedure.
5. For cases involving more than one procedure and different providers who are not involved in the previous procedure, site marking will occur when he/she enters the case, whether the patient is re-draped or not.
  6. Final verification of the site mark should take place during the "time out".

## Exemptions from Site Marking

- A. Interventional procedure cases in which the catheter/instrument insertion site is not predetermined (i.e. pacemaker insertions and cardiac catheterizations).
- B. Midline, single organ procedures and endoscopies without intended laterality.
- C. Interventional radiology cases where
  1. The site has been identified during intra-procedural imaging
  2. Routine nephrostomy tube exchange

## Alternate Marking Conditions

- A. An alternate marking process will be used for cases in which it is technically or anatomically impossible or impractical to mark the site (mucosal surfaces, perineum, premature infants) or for patients who refuse site marking.
  1. Premature infants for whom the mark may cause a permanent tattoo. For side identification, a wrist/ankle band labeled "Operative or Procedural Side" (written with an indelible marker) will be placed on the limb of the correct side.
  2. Minimal access procedures: Minimal access procedures intended to treat a lateralization of an internal organ (percutaneous approach or through a natural orifice), initial the intended site at or near the insertion site. The marked site must remain visible after completion of the skin prep and sterile draping.
  3. Teeth: Indicate the operative tooth name(s) and number on documentation **or** mark the operative tooth (teeth) on the dental radiographs or dental diagram. The documentation, images, and or diagrams are available in the procedure room before the start of the procedure.

4. Lesions and wounds: Site marking is not required if there is an obvious wound or lesion that is the site of the intended procedure. However, if there are multiple wounds or lesions and only some of them are to be treated, and the decision and direction for which ones are to be treated is determined prior to the procedure itself, then the sites to be treated should be marked as soon as possible after the decision is made.

## Site Marking Refusal by the Patient

- A. If a patient refuses the surgical/procedural site marking, the proceduralist will provide the patient with information on why site marking is appropriate and desirable for his/her safety. This allows the patient to make an informed decision.
  1. The proceduralist will validate the surgical/procedural site with the patient and another member of the surgical/procedural team
    - a. For side identification, a wrist/ankle band labeled "Operative or Procedural Side" (written with an indelible marker) will be placed on the limb of the correct side.
  2. The proceduralist will document in the patient's medical record the intended site and the reason why the patient refused site marking.

## Time Out Process

### A. Purpose

1. To conduct a final assessment validating the correct patient, correct procedure, and correct procedural or operative site immediately before starting the invasive procedure or making an incision.

### B. Process

1. Active communication among all relevant members of the surgical/procedure team during the time out. The process is consistently initiated by a designated member of the team and the procedure is not started until all questions or concerns are resolved. See [Attachment 1. AORN Comprehensive Surgical Checklist](#).

## Detailed Requirements

- A. *During the time out, the operative or procedural team must agree, at a minimum, the correct patient, correct procedure, and correct site. Areas may elect to add more elements to the time-out as deemed appropriate by that unit.*
- B. The time-out process will be standardized throughout the organization and will be conducted prior to starting the procedure or making an incision.
- C. The time-out applies to all procedural cases, including cases where the procedural physician is present at the time of the decision to perform the procedure and remains with the patient to the start of the procedure.
- D. There will be a separate time out performed prior to any regional anesthetic involving laterality.

- E. When more than one consent form is completed for more than one procedure being performed on the same patient, a time out will be completed to confirm each subsequent procedure before it is initiated.
- F. For cases involving more than one procedure and different providers, who are not involved in the previous procedure, site marking will occur when he/she enters the case, whether the patient is re-draped or not.
- G. All activities will be suspended (an actual pause), to the extent possible without compromising patient safety, allowing all members to focus on active confirmation of the correct patient, procedure, site, and other critical elements.
- H. A pre-designated member of the team will initiate the time out.
  - 1. All immediate members of the team who will be participating in the procedure at its inception will participate in the time-out (i.e. physicians, anesthesia providers, nurses, technicians, etc.).
  - 2. Interactive verbal communication is expected of all team members. All team members will be allowed to express concerns about the procedure. Concerns will be addressed prior to proceeding with the procedure.
- I. Completion of the time-out must be documented in the patient record validating the correct patient, procedure, and site.

## Compliance Monitoring

- A. All hospital staff and physicians involved in the validation process have the responsibility to ensure patient safety. Failure to follow the Universal Protocol or to resolve issues regarding the performance of the verification, site marking, and the time out must be reported using the appropriate chain of command.
- B. Physicians and hospital staff should follow the department and/or Medical Staff Section chain-of-command for assistance in resolving discrepancies. Refer to the Chain of Command: Paging Response Time and Resolving Questions of Care and or Safety policy.
- C. Non-compliance or resistance to this policy will be reported through the electronic occurrence reporting system for review. All actual and "near miss" situations, where any of the steps of this procedure is not followed or is performed incorrectly, should be reported.
- D. Individual occurrences and aggregate occurrence data will be reviewed by Risk Management and referred to the appropriate Medical Staff and/or Nursing Administration leadership and peer review committee.

## References

1. Joint Commission. (2019). *Hospital Accreditation Program. Chapter: National Patient Safety Goals*. Effective January 2019.? Retrieved from the Joint Commission Website [https://www.jointcommission.org/hap\\_2017\\_npsgs](https://www.jointcommission.org/hap_2017_npsgs)

# Addendum A

## Invasive Procedures Specific to the Universal Protocol

- A. The Universal Protocol applies to the following invasive procedures according to the Universal Protocol: For Surgical and Non-surgical Invasive Procedures policy.
- B. **This list is not all-inclusive:**
1. All taps (i.e., thoracentesis, amniocentesis, paracentesis, pericardiocentesis, pleuracentesis, arthrocentesis, and lumbar puncture).
  2. Invasive pain control procedures (i.e., diagnostic or therapeutic blocks, epidural analgesia).
  3. Invasive radiological procedures (i.e., angiography, arthrogram, biopsy, lymphangiogram, myelogram, splenogram, ventriculogram, Whitaker test).
  4. Endoscopy procedures (i.e., bronchoscopy, colonoscopy, gastroscopy, sigmoidoscopy bronchoscopy, colonoscopy, gastroscopy, sigmoidoscopy, esophageal dilation, ERCP).
  5. Invasive cardio/thoracic procedures. (i.e., angioplasty, cardiac catheterization, implantation of pacer or cardioverter, intra-aortic balloon pump, stent placement, intravascular ultrasound, athrectomy).
  6. Biopsy/excision and drainage or aspiration (i.e., bone marrow, cisternal puncture, breast biopsy).
  7. Chest tube insertions
  8. Central line placement (i.e., CVP, Swan-Ganz).
  9. Peritoneal dialysis catheter insertion
  10. Percutaneous nephrostomy.
  11. IVC (inferior vena cava) filter placement.
  12. Embolization.

Document ID: 019.066

---

### Attachments

[AORN-Comprehensive-Surgical-Check-2019.pdf](#)

### Approval Signatures

Step Description

Approver

Date

System Policy Overnight Committee	Terri Fries: Document Mgmt Spec	8/14/2024
PLC	Joseph Santangelo: Chief Medical, Quality & Safety Officer [AM]	8/2/2024
Med Staff Leads (MEC)	Heather Flint: Sr Spec Lead, Med Staff Services SNE - South Regio	12/28/2023
Med Staff Leads (MEC)	Katryna Glettler: Sr Spec Lead, Med Staff Services SNE - Central Reg	10/6/2023
Med Staff Leads (MEC)	Angela Gee: Sr Spec Lead, Med Staff Services SNE - East Region	10/5/2023
Med Staff Leads (MEC)	Teresa Smith: Executive Office Coordinator	9/26/2023
Document Owner	Joseph Santangelo: Chief Medical, Quality & Safety Officer [AM]	9/26/2023

---

## Applicability

Cadillac Hospital, Charlevoix Hospital, Grayling Hospital, Kalkaska Memorial Health Center, MHC Corporate (Home Health, Dialysis, NMSA, etc.), Manistee Hospital, Munson Medical Center, Otsego Memorial Hospital, Paul Oliver Memorial Hospital

## Standards

No standards are associated with this document



# Radial Artery Access and Care

Magdalena Stewart, DNP, AGPCNP-BC, AGCNS-BC, CCRC  
Todd Adams, DO, FACC



October 2025



## Goal and Objectives

### Goal

The goal for this course is to educate the nurse on radial access anatomy, care, and complications.

### Objectives

1. Describe three benefits and limitations of radial artery access.
2. Differentiate three radial post-procedural complications and their treatments.
3. Explain radial artery patency in relation to radial artery occlusion.

## Background, Benefits, and Limitations of Radial Access

- On August 14<sup>th</sup>, 1992, the first interventional coronary procedure was performed using the radial artery.
- **Radial artery access** is now the **Gold Standard** of practice in the Cath Lab and Interventional Radiology (IR).

Benefits	Limitations
Early ambulation	Prone to vasospasm
Fewer bleeding complications	Arterial vessel size limitations: Women have smaller vessels
Faster discharge rate	Difficult tortuosity
Collateral circulation prevents hand ischemia	Vessel accommodates up to 6fr sheath
Absence of major nerve structures minimizes neurological complications	Radial/brachial anatomical loops

Progress  Page 3 of 32


## Review of Radial Anatomy

The radial artery arises together with the ulnar artery from the bifurcation of the brachial artery just below the bend of the elbow.

It passes along the lateral side of the forearm from the neck of the radius to the styloid process in the wrist and is smaller than the ulnar artery.

**The average diameter of the radial artery is:**

- **2.8mm in females**
- **3.1mm in males**

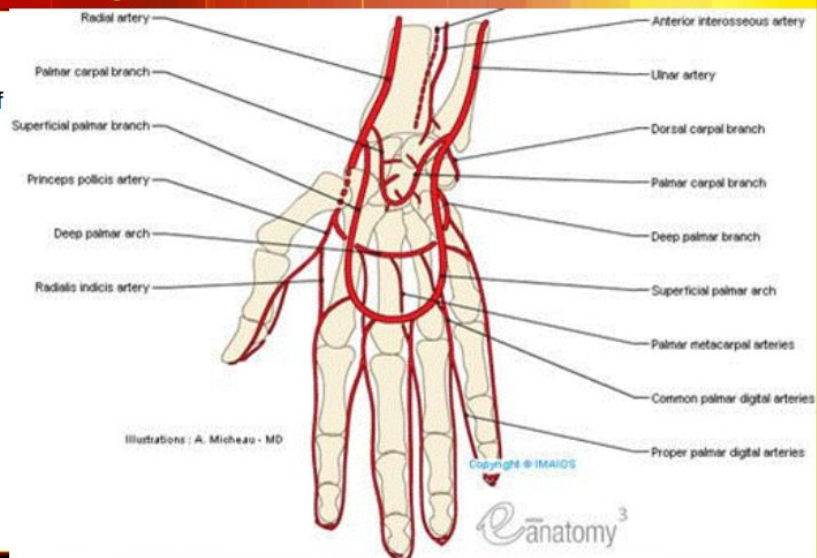

Progress  Page 4 of 32


Image purchased from: <https://www.imaios.com/en/e-anatomy/upper-limb/upper-extremity?mic=ms>

## Anatomical Considerations



### Common radial artery anatomic variants

- **Normal (A)**
- **Other variants:**
  - High take-off radial artery (**B**).
  - Radial and/or brachial loop (**C**).
  - Vessel tortuosity (**D**).
- *Consider abnormal variants as possible limitations to radial access which may increase risk of complications.*

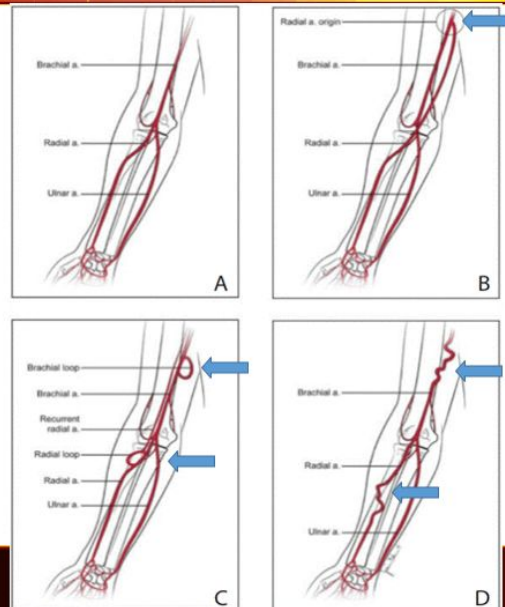

Krishna, H., & Shroff, A. (2018). Ten Common (and Uncommon) Reasons for Unsuccessful Transradial Procedures: [Figure 1]. *Endovascular Today*, 17(11), 50. Retrieved from [https://assets.bmctoday.net/evtoday/pdfs/e11118\\_SF2\\_Shroff.pdf](https://assets.bmctoday.net/evtoday/pdfs/e11118_SF2_Shroff.pdf)

Progress Page 5 of 32

## Pre-procedural Considerations



Pre-procedural care includes:


- Assessment **and** documentation of the radial pulse bilaterally.
- **Clip the wrist** from the base of the thumb, approximately **15cm** towards the antecubital area.
- **Clip the right groin** (may need to use femoral approach, if radial limitations occur).
- Avoid starting an IV within **9cm** of the wrist area.



Progress Page 6 of 32




## Radial Access Sheath Insertion

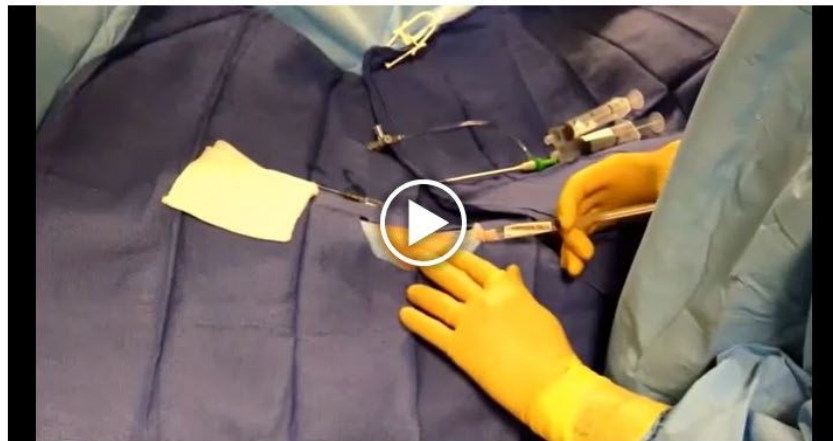

(1½ mins.)

## Radial Access Complications

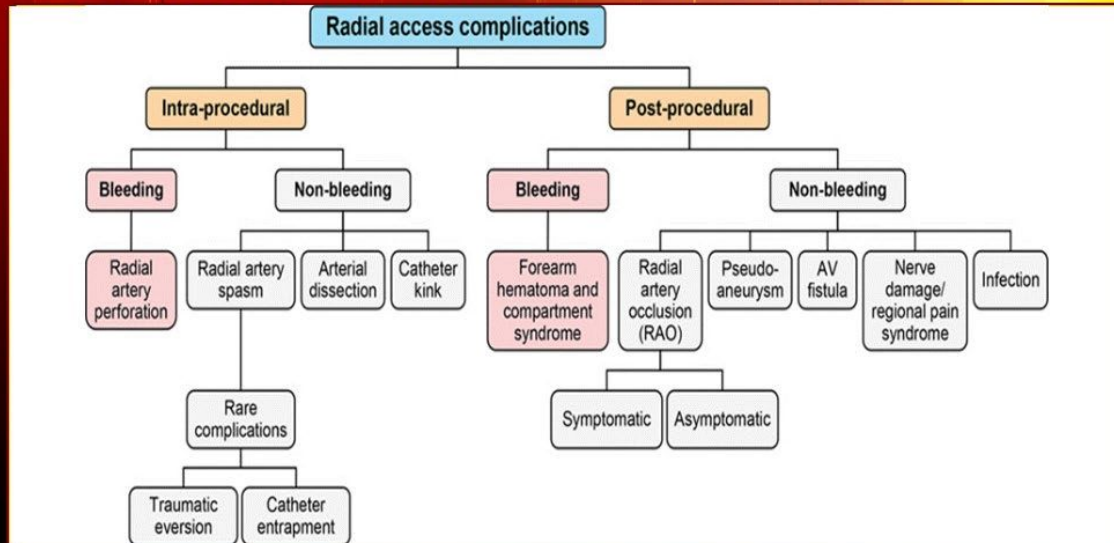

Progress  Page 8 of 32

## Radial Access Care

The compression device is used to apply direct pressure to the radial artery.

Upon receiving patient, verify the radial band is in the correct position (~2mm above the puncture site).

- **Elevate** the arm on a pillow with the site facing up.
- **Place** the **limb-alert** wrist band on the affected hand and leave it on for **2 days** post-procedure.
- Place the **Plethysmography/SpO<sub>2</sub>** monitor on the **affected** hand (index finger or thumb).
  - **Verify patent hemostasis** by occluding the ulnar artery and ensuring blood flow to the hand (plethysmography wave form on monitor).
- **Assess** for signs and symptoms of bleeding, hematoma, pseudo-aneurysm, compartment syndrome, and radial artery occlusion.
- **Control** hypertension.
  - Place the blood pressure (BP) cuff on the **non-procedural** arm.
- **Verify** the type of procedure: Diagnostic vs Intervention
  - **Diagnostic procedure:** Remove 1-2cc of air, **1-hour post-procedure**.
  - **Intervention (PCI, FFR, IVUS, OCT):** Remove 1-2cc of air, **2-hours post-procedure**.
- **Do not leave the radial compression band on the patient for an extended period of time.**

Progress  Page 9 of 32

## Post-Procedural Complications: Re-bleed



### Re-bleeding at the Access Site and Hematoma

- Bleeding can occur from the radial access site or from a small peripheral side branch of the radial artery.
- Local bleeding or hematomas may occur as a result of improper hemostatic device application, device failure, or vessel perforation.

#### What to do?

- **Compression of the radial artery**, *both proximal and distal* to the puncture site must be performed to control both antegrade and retrograde flow from the palmar arch collateral.
- **This can be achieved by** repositioning the hemostatic band or applying manual pressure.
- **If unable to control bleeding** or a growing hematoma at the access site, **occlude the brachial artery**, either manually or with a blood pressure cuff.

## Post-Procedural Complications: Hematoma



### Forearm Hematoma

- Bleeding may also rarely occur from a site on the radial artery remote from the puncture site. It can **occur from a perforation of a small side branch of the radial artery by a guide wire**.
- **If not controlled urgently** and appropriately, forearm hematomas can lead to the development of **compartment syndrome**. The forearm is anatomically susceptible to an increase in pressure, in case of a blood leak, as it has very little room for expansion.

## Forearm Hematoma



### What to do?

- Apply pressure to **occlude** the brachial artery by using the BP cuff to compress the brachial artery.
  - Inflate the BP cuff to **20mmHg above the systolic pressure**.
  - Release the BP cuff pressure for **10-15 seconds every 10 minutes** to allow blood flow to the arm.
- **Assess** for pain, paresthesia, pallor, and pulselessness of the hand.
- **Protamine** can be used for Heparin reversal.
- **Control hypertension**, attain pain management, and closely monitor the distal perfusion bed with plethysmography.
- Assess the hematoma every 15 mins. by **measuring it with a measuring tape. Mark the borders with a marker** to check if the hematoma is growing.
- **Suspect compartment syndrome?** Consult a vascular surgeon.

## Compartment Syndrome



This is a **rare** complication of radial artery catheterization. ***If not identified and treated emergently, it can lead to profound disability or limb loss.***

### Compartment syndrome is an **EMERGENCY!**

Greater than expected **pain** is the earliest and most reliable indicator.

- Escalating pain unrelieved by immobilization and requiring increasing analgesics should illicit high suspicion.

A **swollen and tense** compartment is a direct manifestation of increased pressure.

An **abnormal sensation**, feeling like “pins and needles” and tingling, can be in the arm and hand.

#### **Late indicators**

- **Decreased pulses.**
- **Absence of pain** - due to tissue ischemia and necrosis or nerve injury.

## Post-Procedural Complications - Pseudoaneurysm



### Pseudoaneurysm

- Rarely occurs at the radial artery access site.
- Should be suspected in the presence of **pulsatile swelling at the access site**.
- **Often painless**; however, some patients can have associated discomfort.
- **Risk factors**: systemic anticoagulation, inadequate compression post-procedure, infection, and multiple arterial punctures.

**Diagnosis is confirmed by ultrasound.**

### What to do?

- **Apply pressure** to the **brachial** artery **and notify the provider**.
- **Management options ordered by provider**: compression with a radial hemostasis device, thrombin injection, ultrasound-guided compression, or surgical repair.

## Post-Procedural Complications - Radial Artery Occlusion



### Radial Artery Occlusion (RAO)

- Occurs in 1-12% of cases.
- **Often asymptomatic** and goes unnoticed.
- **Limits use of the radial artery for**: future cardiac catheterizations, use as a conduit in patients undergoing coronary artery bypass graft surgery, or for creation of an arteriovenous fistula in patients with end-stage renal disease.
- Hand ischemia is rare, but may occur.

## Factors Impacting the Risk of RAO



### Pre-procedural risk factors

- Elevated creatinine
- Female
- Low body weight
- Diabetes

### Intra-procedural risk factors

- Artery to sheath ratio >1
- Vasospasm
- Longer procedure time

### Post-procedural risk factors

- Longer compression
- Too much compression limiting blood flow through radial artery

## Radial Artery Occlusion Risk Reduction



Factors that decrease the risk of RAO:

- Smaller catheters
- Heparin use during procedure
- Timely sheath removal
- **Patent hemostasis!!!**
- Short duration of compressive device

## What is Patent Hemostasis?



**Patent hemostasis** is the technique of maintaining radial artery flow through guided artery compression during hemostasis.

- After the procedure is completed, the compression band is applied and 15-20cc of air is injected to exhibit pressure on the radial artery puncture site by the Cath Lab.
- The radial sheath is removed and no exterior bleeding should be observed at the arteriotomy (puncture) site.
- This volume of air typically creates radial artery total or partial collapse. At this point, slow balloon deflation (1cc/second) is performed until a small jet of bleeding is observed at the skin puncture site. In order to stop it, a quick insertion of 2cc of air is performed.

## Radial Artery Patency (Patent Hemostasis)



**Using a pulse oximetry waveform, radial artery patency should be assessed:**

- Immediately after application of the compression device.
- On arrival to recovery room/inpatient unit.
- Whenever there is an increase in amount of air in the compression or adjustments to the compression band.
- After removal of the compression band.
- At the time of discharge.


## How to Check Patent Hemostasis

- Patency of the radial artery is checked with a **reversed Barbeau's test**.
- Place the oximetry pulse detector on the patient's thumb or index finger on the affected hand. With the balloon inflated on the top of the radial artery, **simultaneous manual compression should be applied to collapse the ulnar artery**.
- If the inflated balloon has **too much pressure**, causing radial artery collapse, **the plethysmography pulse waveform will be flat**; in other words, there is no "flow" pulse/flow reaching the detector. In that case, an additional *1cc should be aspirated* from the balloon with the goal to reestablish flow through the radial artery.

Progress  Page 20 of 32

## What to Do for No-Flow on Pulse Oximetry

- If **no-flow** is identified, **remove 1-2cc of air** from the band until the flow is restored and patent hemostasis is achieved.
- If **bleeding occurs** and **unable** to maintain hemostatis, re-check in 15 minutes.
- If **no-flow is identified after the band is removed**, **immediately notify the provider**.
- Document patent hemostasis in IView.

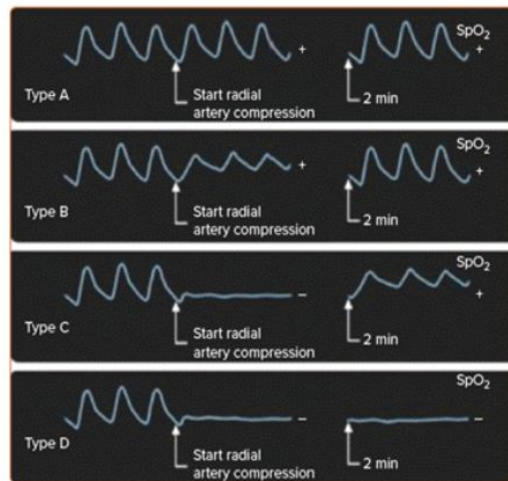

A,B, and C show patent hemostasis

D indicated no flow

Progress  Page 21 of 32

## Site Assessment Post-Procedure



Thoroughly assess the radial access site for:

- Bleeding or oozing
- Hematoma formation
- Pain or tenderness
- Bruising/Discoloration

Perform neurovascular checks and document:

- Capillary refill
- Skin temperature and color: Compare with contralateral hand
- Radial and ulnar pulses: Presence, strength, and symmetry
- Sensation and motor function: Assess fingers for movement and any numbness/tingling
- Reversed Barbeau Test post-procedure to ensure collateral circulation


## Post-Procedure Site Documentation



- Assess site immediately after arrival from the procedure.
- Verify the time and that the radial compression band was applied.
- Follow provider orders for frequency of site assessment.
- Assess site immediately before and immediately after any activity.
- Document the site assessment in PowerChart.



## Sheath/Site Documentation

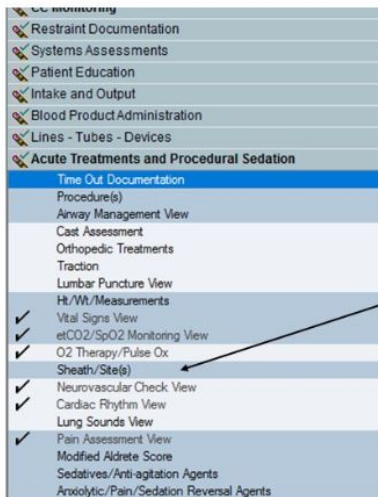

- Document sheath sites and neurovascular status in the Sheath/Site(s) section of the "Acute Treatments and Procedural Sedation" band in iView.

## Sheath/Site Documentation (con't)



- Add a dynamic group for each site

- Select the correct site and choose "TR band" for a radial site with a band in place

Label: <Sheath Start Date/Time>-Radial Artery Right TR Band <Sheath Intervention Site Detail>

Brachial Artery Right  
Brachial Artery Left  
Brachial Vein Right  
Brachial Vein Left  
Femoral Artery Right  
Femoral Artery Left  
Femoral Vein Right  
Femoral Vein Left  
Popliteal Artery Right  
Popliteal Artery Left  
Popliteal Vein Right  
Popliteal Vein Left  
**Radial Artery Right**  
Radial Artery Left  
Tibial Artery Right  
Tibial Artery Left  
Tibial Vein Right  
Tibial Vein Left  
Other

Sheath IV Gauge

4 French  
5 French  
6 French  
7 French  
8 French  
9 French  
10 French  
11 French  
12 French  
14 French  
**TR Band**  
Other

## Sheath/Site Documentation (con't)

- Document the assessment including:
  - Site condition
  - Presence of a closure device
  - Compression activity/band
  - Drainage
  - Site interventions
- **NOTE:** A TR band is NOT a closure device.
- With each site assessment, document a neurovascular check of the affected limb.

Sheath/Site(s)	
9/24/2025 10:23 Radial Artery Right 6 Fren...	
Activity, Sheath/Site	Assessm...
Site Check, Sheath/Site	WDL
Variance, Sheath/Site	
Closure Device, Sheath	No
Site Drainage, Sheath/Site	none
Fluid Infusing, Sheath	
Site Dressing, Sheath/Site	Securem...
Site Interventions, Sheath/Site	Radial b...
Manual Pressure Duration, Sheath/Site	minute(s)
Compression Activity, Sheath/Site	in positi...
Air Add/Removed, Sheath/Site	CC
Compression	
Hemostasis Achieved, Sheath/Site	
Patient Response, Sheath/Site	Well
Additional Information, Sheath/Site	
Neurovascular Check View	

## Summary

- Radial approach is the gold standard of practice in the Cath Lab.
- It allows for early mobilization, increases patient satisfaction, and decreases bleeding complications.
- Nursing interventions include awareness and prevention of complications.
- A rare complication of radial access is compartment syndrome.
- With the increase in radial use, RAO is a potential concern with permanent consequences.
- Patent hemostasis is considered best practice to prevent RAO.

**For any questions or concerns, please contact the Cath Lab Clinical Nurse Specialist.**

## Case Study #1



Patient: John D., 67-year-old male

Procedure: Coronary angiography via right radial artery

Post-procedure orders:

- Radial compression band applied
- Vital signs Q15 minutes X 1 hour, then Q30 minutes X 2 hours
- Assess neurovascular status and site per protocol

### Situation:

One hour post-procedure, the nurse notes that the patient's right hand is cooler than the left, and capillary refill is sluggish. The radial pulse is weak but present. The compression band is still inflated at the same pressure as it was post-procedure.

Progress  Page 28 of 32

## Case Study #1 Questions



### Question 1:

What is the nurse's priority action in response to the assessment findings?

- Document findings and continue monitoring
- Notify the provider immediately
- Deflate the radial band slightly and reassess perfusion
- Apply a warm compress to the affected hand

### Question 2:

Which of the following is a critical nursing intervention during the first hour after radial artery procedures?

- Encourage full mobility to prevent stiffness
- Frequently assess for signs of bleeding and neurovascular compromise
- Apply ice packs to prevent inflammation
- Encourage the patient to flex the wrist to promote circulation

Progress  Page 29 of 32

## Case Study #2



Patient: Maria L., 58-year-old female

Procedure: Subclavian artery stent via left radial access

Post-procedure orders:

- Radial compression band to be weaned off over 2 hours
- Monitor access site for bleeding, swelling, and hematoma
- Patient instructed to report tingling or numbness

### Situation:

90 minutes post-procedure, the nurse begins deflating the radial band as per protocol. As air is released, the patient reports feeling a "warm, wet sensation" at her wrist. On inspection, there is oozing at the site.

## Case Study #2 Questions



### Question 1:

What is the most appropriate immediate response by the nurse?

- Continue deflating the band
- Re-inflate the band slightly and apply direct pressure
- Remove the band and apply a gauze dressing
- Notify the provider and document the finding

### Question 2:


Which patient complaint would be most concerning during radial band monitoring?

- "My hand feels cold and numb"
- "This band is tight, but not painful"
- "I feel tired and want to sleep"
- "I'm feeling a little thirsty"

## References



- Bourassa M. G. (2005). The history of cardiac catheterization. *The Canadian journal of cardiology*, 21(12), 1011–1014.
- Fischman D, et al. (2021) "Up in Arms" Making the Argument for Broadening the Use of the Radial Artery. *Journal of American College of Cardiology Interventions*. (8) 917–918. <https://doi.org/10.1016/j.jcin.2021.02.023>
- Krishna, H., & Shroff, A. (2018). Ten Common (and Uncommon) Reasons for Unsuccessful Transradial Procedures: Understanding the limitations of radial access is key to optimal application. [Review of *Ten Common (and Uncommon) Reasons for Unsuccessful Transradial Procedures Understanding the limitations of radial access is key to optimal application*.] Figure 1., *Endovascular Today*, 17(11), 50. [https://assets.bmctoday.net/evtoday/pdfs/et1118\\_SF2\\_Shroff.pdf](https://assets.bmctoday.net/evtoday/pdfs/et1118_SF2_Shroff.pdf)
- Mitchell, M. D., Hong, J. A., Lee, B. Y., Umscheid, C. A., Bartsch, S. M., & Don, C. W. (2012). Systematic review and cost–benefit analysis of radial artery access for coronary angiography and intervention. *Circulation: Cardiovascular Quality and Outcomes*, 5(4), 454–462.
- Pristipino, C., Trani, C., Nazzaro, M. S., Berni, A., Patti, G., Patrizi, R., ... & Richichi, G. (2009). Major improvement of percutaneous cardiovascular procedure outcomes with radial artery catheterization: results from the PREVAIL study. *Heart*, 95(6), 476–482.
- Roy, S., Kabach, M., Patel, D. B., Guzman, L. A., & Jovin, I. S. (2022). Radial artery access complications: prevention, diagnosis and management. *Cardiovascular Revascularization Medicine*, 40, 163–171.
- Sandoval, Y., Bell, M. R., & Gulati, R. (2019). Transradial artery access complications. *Circulation: Cardiovascular Interventions*, 12(11), e007386.
- Shroff, A., Pinto, D. (2021). Vascular access, management and closure. Best practices. The Society for Cardiovascular Angiography and Interventions (SCAI)



# Femoral Post Sheath Removal Care

Magdalena Stewart, DNP, AGPCNP-BC, AGCNS-BC, CCRC

December 2025



## Goal and Objectives

### Goal

To educate health care providers in the care of the patient femoral post sheath removal.


### Objectives

1. Identify vascular anatomy.
2. State the process of hemostasis.
3. Define five complications that may occur femoral post sheath removal.
4. Identify potential complications associated with closure/compression devices.
5. State two nursing considerations for identified complications.



## Vascular Anatomy

Identify the nerve, artery, vein, and ligament structures in the groin area.

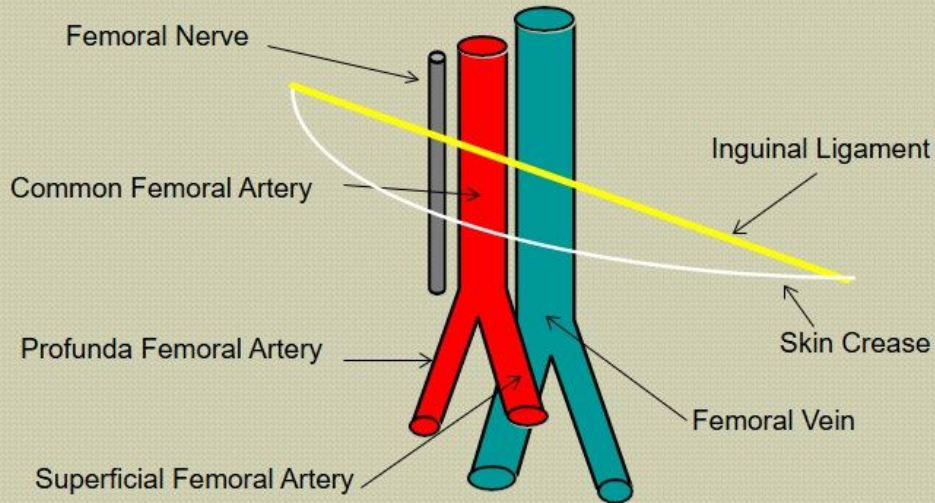


Progress



## Vascular Anatomy Relevant to the Sheath Insertion Site


The arterial stick should be placed approximately 3 cm below the inguinal ligament and directly over the femoral artery pulse.

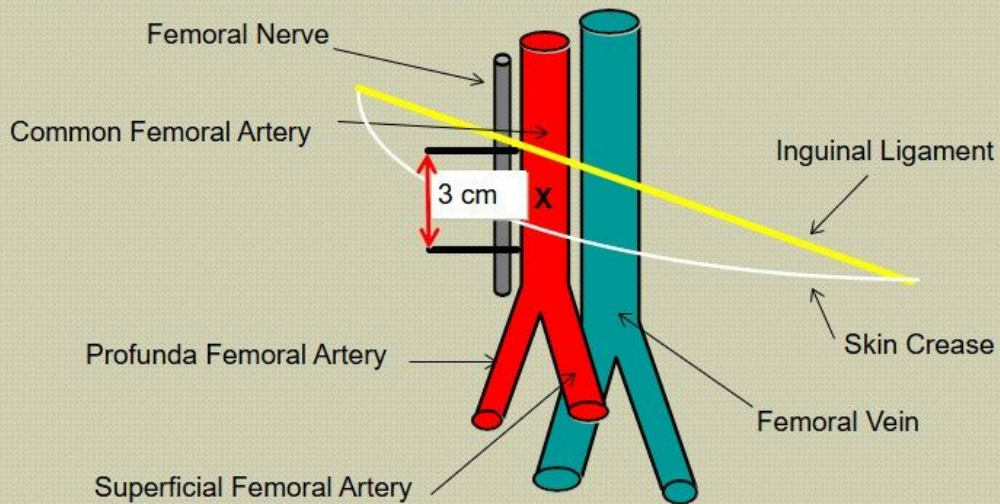

Progress


## Arterial Puncture

If the arterial puncture is too high or too low, it may result in vascular complications. Review the correct position for puncture below.

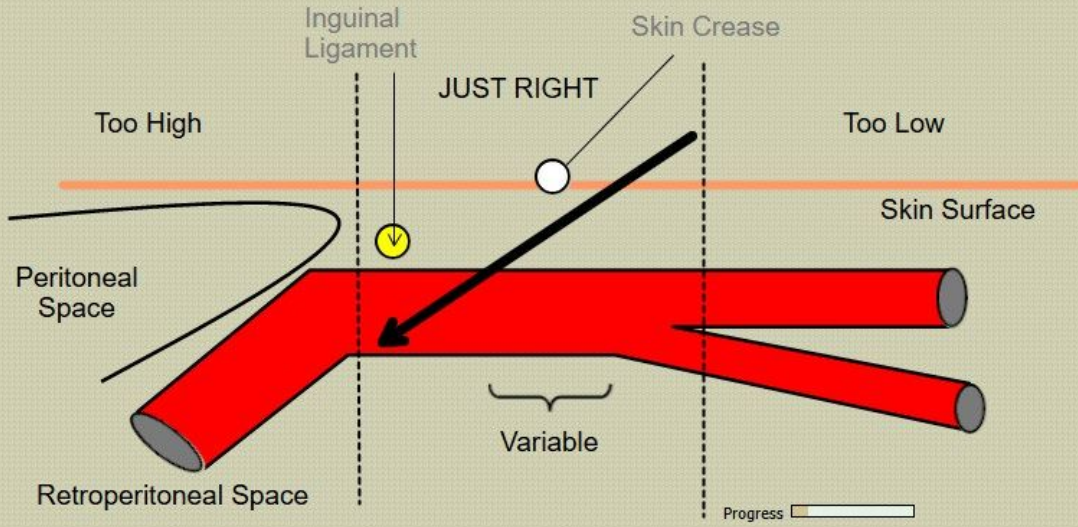


## The Hemostasis Process

This is the normal hemostasis process. The process can be disrupted by certain drugs such as heparin and Integrilin.

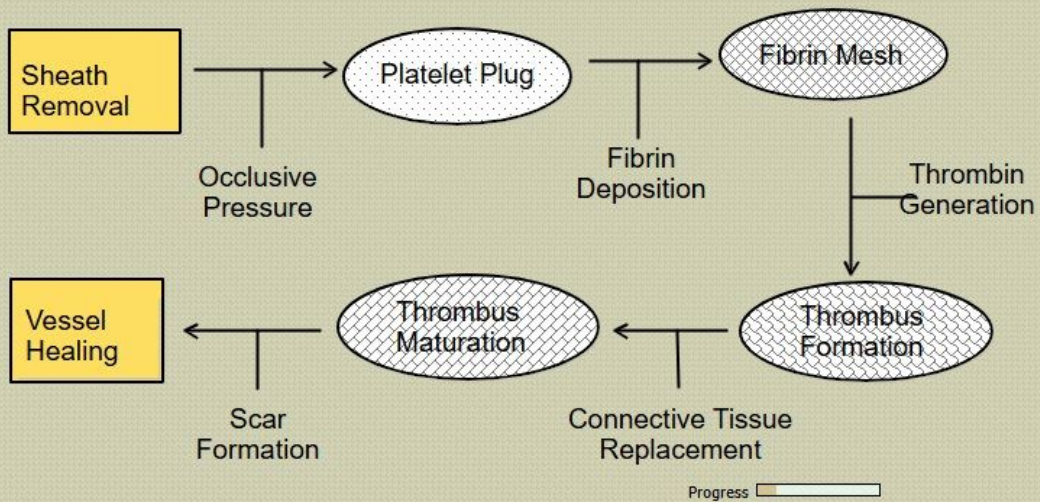


# Hemostasis

Manual pressure should be applied 2-3 cm above the skin puncture to achieve hemostasis.

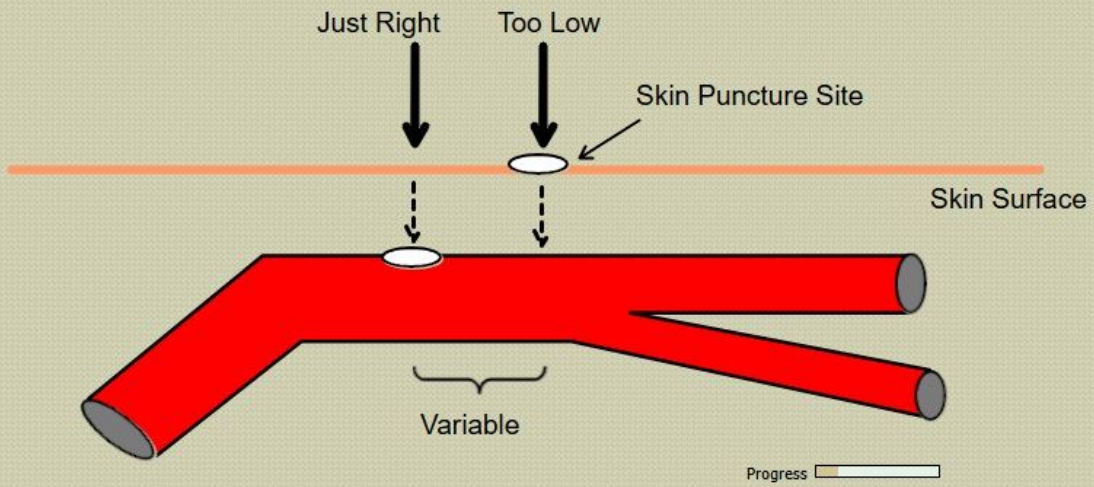

# Hemostasis (cont.)

Vascular anatomy may be displaced depending on the weight of the patient.

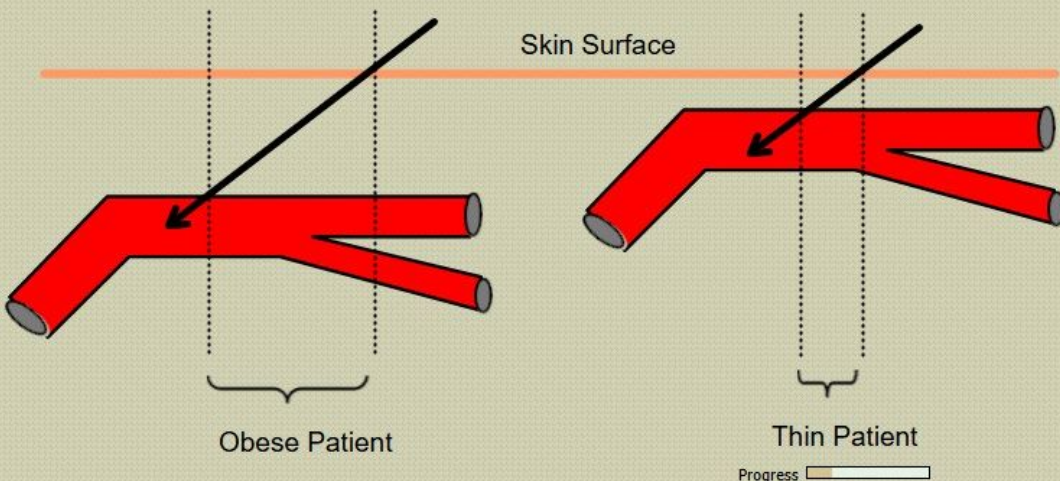



## Post Sheath Pull: Potential Vascular Complications

- Vessel thrombosis and dissection
- Bleeding
- Re-bleeding
- Femoral hematoma
- Retroperitoneal hemorrhage
- Pseudoaneurysm
- Arteriovenous fistula
- Atheroembolism


If any of the above complications occur, contact:  
Cardiac Cath Lab - 231-935-9578  
or the "neuro-on-call" if IR case

Progress



## Vascular Complications: Vessel Thrombosis and Dissection

Blood flow may be inhibited by a thrombus or dissection.

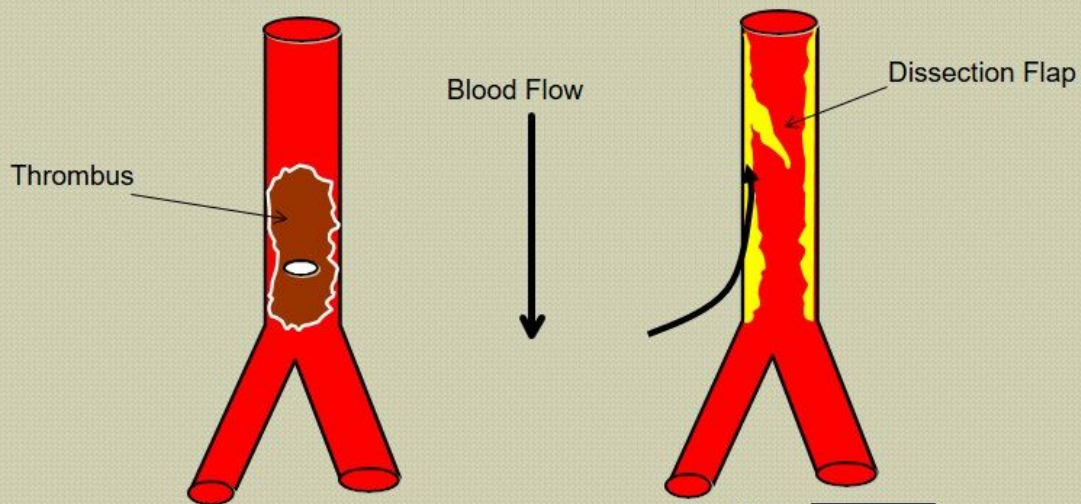



## Vascular Complications: Vessel Thrombosis and Dissection *(cont.)*

### Key Points

- Femoral artery thrombosis is rare and typically occurs in patients with small arterial lumens. Examples: peripheral vascular disease (PVD), diabetes mellitus (DM), and female gender.
- Dissection usually occurs in the setting of PVD or difficult arterial access.
- Patients commonly complain of leg pain or numbness.
- Physical exam reveals diminished or absent pulses.
- Rapid recognition is critical to avoid irreversible limb ischemia.
- Doppler ultrasound can be diagnostic.
- Urgent revascularization (surgical or percutaneous) is the treatment of choice.


Progress



## Vascular Complications: Re-Bleeding

A re-bleed is uncontrolled bleeding from the puncture site.

- It is possible for the Hematocrit to drop by  $\geq 10\%$  and the hemoglobin to drop by  $\geq 3$  g/dL.
- The patient may require a transfusion.

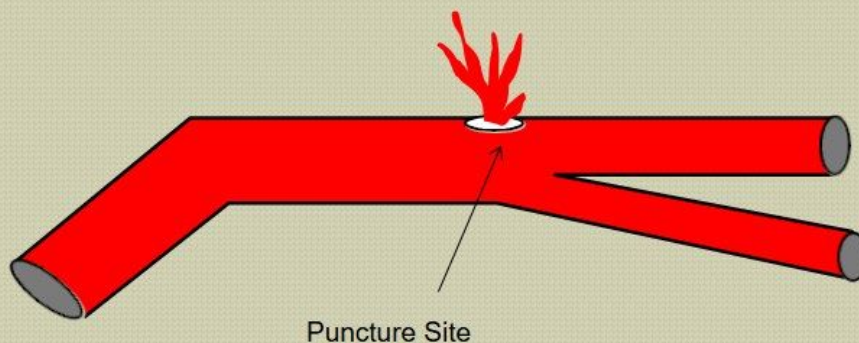

Progress



## Nursing Considerations: Re-Bleeding

- Assess distal pulse prior to compression.
- Apply gloves and palpate artery just superior to puncture site.
- **Apply manual pressure above the site for a minimum of 20 minutes. No peeking!**
- Compression should be forceful enough to prevent bleeding, oozing, and hematoma formation.
- Delegate someone to call the cardiology provider.
- After bleeding stops, assess for hematoma.
- After hemostasis, restart bed rest and site checks per protocol.
- Document in a Focus Note in PowerChart.
- Assess distal pulses.
- Check Hgb/Hct, if indicated.




Progress



## Vascular Complications: Hematoma

A hematoma is a collection of blood in the soft tissues of the upper thigh causing a tender mass of variable size.

- It is possible for the Hematocrit to drop by  $\geq 10\%$  and the hemoglobin to drop by  $\geq 3$  g/dL.
- The patient may require a transfusion.

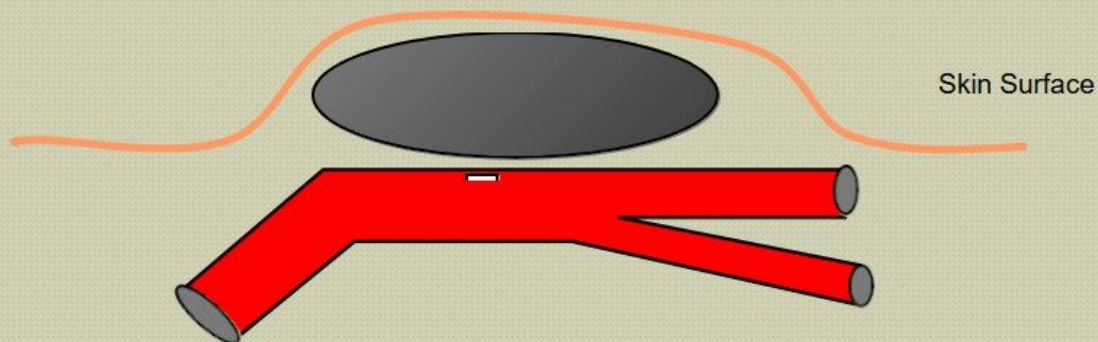


Progress

## Vascular Complications: Hematoma *(cont.)*

### Risk Factors:


- Female gender
- Low platelet count
- Operator technique - inaccurate puncture of common femoral artery; number of arterial punctures
- Anticoagulation and/or platelet inhibitors
- Sheath size
- Delayed sheath pull
- Sheath pull technique
- Noncompliant patient or patient unable to comply with bed rest protocol

Progress 

## Vascular Complications: Hematoma *(cont.)*

### Key Points:

- Hematomas can occur at any time before or after sheath removal.
- Measure (by palpation or imaging) and document the maximal dimension of the hematoma in centimeters.
- Immediate treatment includes correct manual compression. Do not “mash on” or massage the hematoma as this can cause damage to the vessel.
- Serial Hgb measurements and blood transfusions as needed. These are the treatments of choice.
- 1 - 2 weeks is required to reabsorb the hematoma and the patient should be warned about normal changes in the hematoma's appearance.
- Femoral nerve compression can occur from large hematomas.
- Surgical drainage is rarely needed.
- **Deaths do occur from hematomas - they must be respected.**

Progress 

## Nursing Considerations: Hematoma

- Assess distal pulse prior to compression.
- Apply gloves and palpate artery just superior to puncture site.
- **Apply manual pressure above the site for minimum of 20 minutes. No peeking!**
- Compression should be forceful enough to prevent increased hematoma formation, while maintaining distal pulses.
- Delegate someone to call the cardiology provider.
- Mark site: measure in centimeters.
- In PowerChart, document both a Focus Note and the hematoma size in Iview.
- Check Hgb/Hct, if indicated.



Progress

## Nursing Considerations: Manual Compression Technique



Wrong Techniques



Correct Technique




Progress



## Vascular Complications: Retroperitoneal Hemorrhage

A retroperitoneal hemorrhage is a hematoma extending into the retroperitoneal space that usually occurs from arterial puncture above the inguinal ligament.

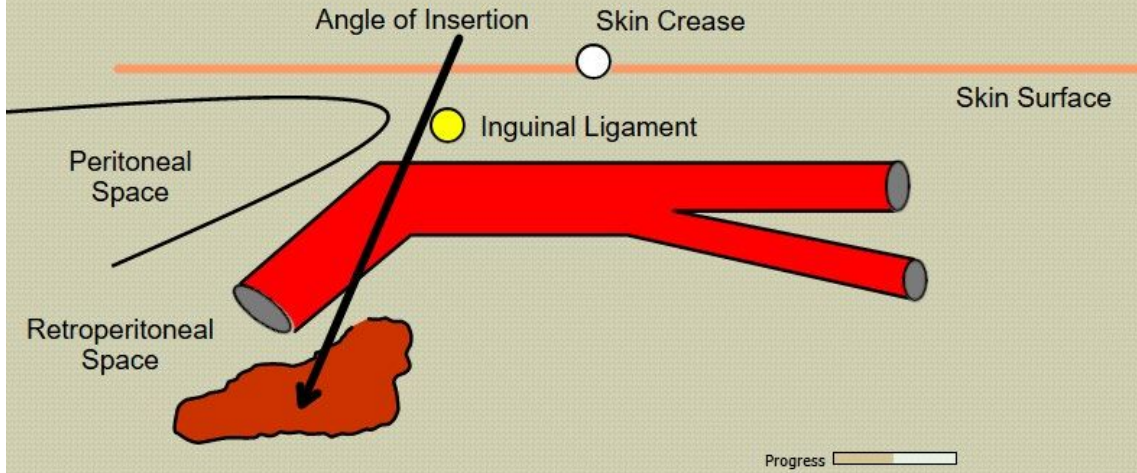

Progress



## Vascular Complications: Retroperitoneal Hemorrhage *(cont.)*

### Risk Factors:

- Female gender
- Low platelet count
- Improper operator technique: a “high” stick above the inguinal ligament or a puncture through the back wall of the artery
- Anticoagulation and platelet inhibitors
- Sheath size
- Delayed sheath removal


Progress



## Vascular Complications: Retroperitoneal Hemorrhage *(cont.)*

### Key Points:

- This type of bleeding is not evident from the surface.
- Symptoms include hypotension, abdominal pain, and ipsilateral flank pain.
- Physical exam may reveal a palpable mass with discoloration over the flank or abdomen.
- Marked anemia can occur from blood loss.
- **This is a life-threatening situation!**
- CT scanning is the diagnostic test of choice.
- Treatment usually involves stopping anticoagulants, bed rest, and blood transfusion.


Progress 




## Vascular Complications: Pseudoaneurysm

A pseudoaneurysm is an interruption of the artery wall from the femoral artery puncture that does not thrombose when arterial sheaths are removed. This interruption in the arterial wall, caused by the original puncture, allows blood to jet back and forth from the bloodstream to the pouch. The aneurysm is termed "false." It does not involve any layers of the vessel wall as found with a true aneurysm.

"False" aneurysms can be masked by a hematoma and may rupture at any time. They continue to expand because they lack elastic fibers.

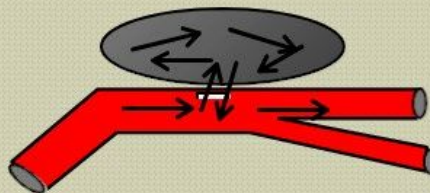


Progress 



## Vascular Complications: Pseudoaneurysm *(cont.)*

### Risk Factors:

- Anticoagulation and platelet inhibitors.
- Obesity - causes difficulty in maintaining direct pressure.
- Advanced age - causes loss of tissue elasticity.
- Atherosclerotic occlusive disease.
- Increased sheath size - creates larger vascular interruption.
- Improper operator technique.
- Thrombolytic therapy - interrupts previously achieved hemostasis.
- Infection - impairs healing at the site of hemostasis.

Progress 



## Vascular Complications: Pseudoaneurysm *(cont.)*

### Key Points:

- Physical exam reveals a pulsatile mass with a bruit auscultated superior to the puncture site. Bruits are heard when an artery is partially obstructed causing turbulent blood flow.
- Listen for bruits with the **bell** of the stethoscope **held lightly** against the skin.



Progress 



## Vascular Complications: Pseudoaneurysm *(cont.)*

### Key Points:


- Duplex ultrasound scanning allows a measure of size as well as distinction from intravenous fistula.
- There is a risk of enlargement and ultimate rupture if not detected and treated.
- Pseudoaneurysms smaller than 3 cm tend to close spontaneously or with compression.
- Those larger than 3 cm require alternative methods:
  - Ultrasound guided compression
  - Thrombin injection
  - Surgical repair

Progress



## Vascular Complications: Arteriovenous Fistula

An arteriovenous fistula is an abnormal connection between an artery and a vein which forms when ongoing bleeding from the arterial puncture site decompresses into an adjacent venous structure.

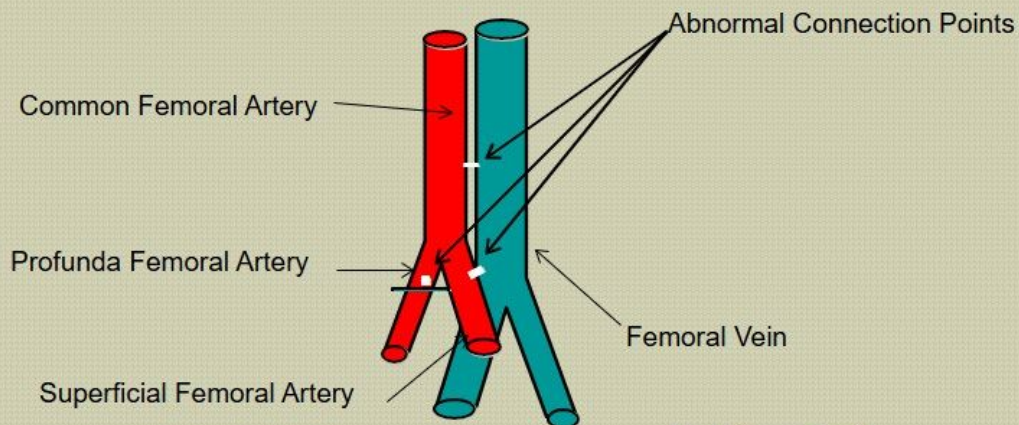


Progress



## Vascular Complications: Arteriovenous Fistula *(cont.)*

### Risk Factors:

- Anticoagulation and platelet inhibitors.
- Female gender.
- Obesity - causes difficulty in maintaining direct pressure.
- Advanced age - causes loss of tissue elasticity.
- Atherosclerotic occlusive disease.
- Increased sheath size - creates larger vascular interruption.
- Improper operator technique.
- Poor sheath pull technique.
- Thrombolytic therapy - interrupts previously achieved hemostasis.
- Infection - impairs healing at the site of hemostasis.


Progress 



## Vascular Complications: Arteriovenous Fistula *(cont.)*

### Key Points:



- AV fistulas may not present for days.
- Physical exam reveals a to-and-fro murmur or continuous bruit.
- AV fistulas tend to enlarge with time.
- If they do not close spontaneously after 2 - 4 weeks, surgical repair is indicated.

Progress 



## Vascular Complications: Atheroembolism

- The release of cholesterol crystals and other microscopic debris from the aorta after catheter manipulation results in mechanical trauma to friable atheromatous plaques.
- Distal embolization may occur to the lower extremities and abdominal viscera.

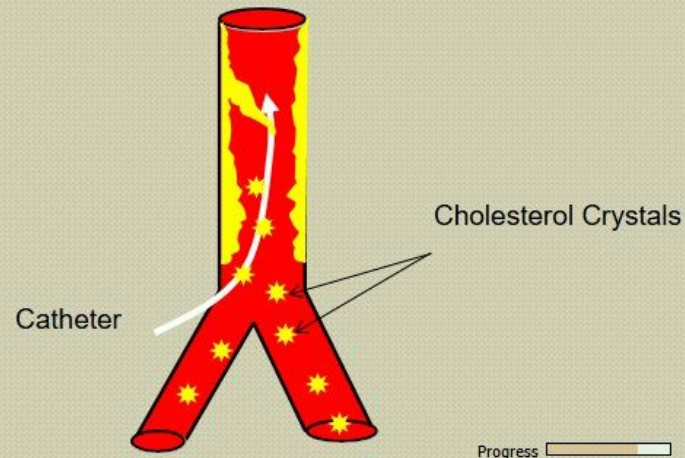

## Vascular Complications: Atheroembolism *(cont.)*

### Key Points:

- Physical exam may reveal a cyanotic foot in the case of microemboli and signs of limb ischemia in the case of macroemboli.
- Renal failure can occur if the renal arterial bed is involved.
- Distal gangrene and death can occur, in extreme cases.
- The onset is often insidious and can take days to months to become evident.
- Management is variable depending on the severity.



## Compression and Closure Devices

Compression of an artery and the use of closure devices must be deployed correctly and appropriately to decrease the risks of vascular complications. You may need to perform manual pressure or utilize a Femostop if the patient re-bleeds.

### Compression options:

- Manual pressure
- Femostop

### Closure devices:

- Angioseal
- Perclose
- Vascade



Femostop

**Note: Femostops should not be used on patients with peripheral vascular disease.**

Progress



## Compression and Closure Devices *(cont.)*

### Key Points:


- Multiple studies have shown that the lowest complication rates occur with correctly applied manual pressure.
- Incorrect application of compression devices is a common error in post sheath removal care.
- Bleeding, despite a compression device (Femostop), mandates removal of the device and manual control of the hemorrhage.
- Closure devices are not a substitute for close observation and have their own set of possible complications.
- If a closure device fails, manual control of the hemorrhage is needed.

Progress



## Nursing Considerations: Femoral Post Sheath Removal

- Post procedure checks per protocol (every 15 min x 4, every 30 min x 4, every 1 hour until stable, then prn).
- Document post procedure checks in IView.
- Per Interventional Order Set:
  - Bed rest and activity guidelines
  - PRN medications for back pain or discomfort
  - IV fluid discontinuation or restart
  - Ambulate at least 1 hour prior to discharge
- Patient education on re-bleeding and groin care.
- When receiving the patient, always check the site together with the recovery nurse before he/she leaves the room.


Progress 



## Nursing Considerations: Hypotension

### Systolic BP < 90 mmHg:

- Increase IV fluids: Give 250 ml 0.9 NS bolus and call cardiologist for further orders.
- Give 0.5 mg – 1 mg Atropine IVP if suspect cause is due to vasovagal stimulation.
- Call cardiology provider if hypotension does not resolve quickly.
- Assess for signs of retroperitoneal bleeding (i.e., flank pain, increased heart rate, decreased blood pressure).
- Assess for signs of a pseudoaneurysm (i.e., auscultated bruit).

Progress 



## Nursing Considerations: Bradycardia Due to Vasovagal Stimulation

- Give 0.5 mg – 1 mg Atropine IVP.
- Treat cause of vasovagal response (i.e., anti-emetics for nausea/vomiting).
- Increase IV fluids for associated hypotension.
- Call cardiology provider if bradycardia does not resolve quickly or if ACLS treatment is required.
- Assess hand/Femostop positioning and adjust.

Progress



## Nursing Considerations: Loss of Pedal Pulses

- Assess affected limb for pain, coolness, or mottling.
- Attempt to find pulse with a Doppler.
- Adjust amount of pressure to obtain a balance between hemostasis and adequate pulses.
- Call cardiology provider.

Progress



## Patient Education: Femoral Post Procedure Instructions

- Can elevate HOB 30 degrees 1 hour post procedure. May log roll patient to affected side in 1 hour.
- Vital signs/groin assessment checks - every 15 minutes x 4, then every 30 minutes x 4, then every 1 hour until stable, and prn.
- Notify RN of any pain, change in sensation, warmth, or bleeding at the groin site.
- Notify RN of any signs and symptoms of angina: chest discomfort; jaw, neck, arm, or shoulder pain; shortness of breath; sweating; nausea; dizziness or lightheadedness.

Progress



## Patient Education: Femoral Post Procedure Instructions *(cont.)*

- The RN may administer an anti-emetic agent to prevent vomiting which causes unnecessary strain at the groin site.
- Refrain from activities that will cause strain to the groin site; for example, do not lift head, raise up on elbows, or bend knees when repositioning.

Progress



## References

- American College of Cardiology Foundation. (2008). CathPCI Registry, NCDR CathPCI Registry v. 4.3.1. Coder's Data Dictionary. pp. 76-78.
- Munson Medical Center Procedures. (2024). Arterial and venous sheath removal. Lippincott Procedures.
- Munson Medical Center Procedures. (2024). Femoral compression device use. Lippincott Procedures.
- Munson Medical Center Procedures. (2024). Left heart catheterization post procedure care. Lippincott Procedures.
- Munson Medical Center PolicyStat. (2023). Arterial/Venous Sheath Management.

Progress



**Procedure:** Bair Hugger Warming Blanket (MUNSON)  
**Checklist:** Bair Hugger Warming Blanket (MUNSON)  
**Evaluator's Name:** \_\_\_\_\_ **Examinee's Name:** \_\_\_\_\_  
**Evaluator's ID:** \_\_\_\_\_ **Examinee's ID:** \_\_\_\_\_  
**Evaluator's Dept:** \_\_\_\_\_ **Examinee's Dept:** \_\_\_\_\_  
**Date:** \_\_\_\_\_ **Meets criteria/Does not meet criteria:** \_\_\_\_\_

**Select Evaluation Method:**  
 Clinical Observation  Documentation Review  
 Demonstration  Verbalization

**Bair Hugger Warming Blanket (MUNSON)**

<b>Objective: To safely apply Bair Hugger Warming Blanket to patient.</b>
<b>***State what population-served considerations you made (or would make) in providing care for the patient.***</b>
<input type="checkbox"/> Place Bair Hugger blanket on patient with the perforated side (side with the small holes) against the patient's skin.
<input type="checkbox"/> Plug unit in and turn on to desired temperature setting (low, medium or high).
<input type="checkbox"/> Let unit run for about 1 minute to let air warm up.
<input type="checkbox"/> Insert hose into the port on the blanket using a twisting motion to ensure a snug fit. (Do not blow air directly from hose onto patient.)
<input type="checkbox"/> Place a cotton blanket over Bair Hugger blanket to maximize effectiveness.
<input type="checkbox"/> Monitor patient's temperature every 10-20 minutes and adjust temperature setting on Bair Hugger as needed.
<b>Competence in the task will be recognized according to achievement of indicators listed.</b>
<b>Need for competency identified by: new equipment/procedure and job description.</b>
<b>Method of validation: return demonstration, direct observation with patient by peer/manager.</b>
<b>Action plan/comment developed for all findings rated "not met":</b>



# Broselow™ Pediatric Resuscitation Cart

Duane Croel  
Lauren Holland  
Marissa Loud, MMC  
Marta Wiesen, MMC

December 2025



## Goal and Objectives

### Goal

The purpose of this course is to familiarize clinicians with the Broselow™ system and where supplies are located on the pediatric resuscitation cart.

### Objectives:

1. Describe how to call a Code Blue - Pediatric Medical Emergency.
2. Describe how to use the Broselow™ pediatric emergency tape.
3. Identify the location of Broselow™ carts throughout your hospital.
4. Identify the location of specific pediatric equipment in the Broselow™ Pediatric Resuscitation Cart based on the child's weight.

## Code Blue - Pediatric Medical Emergency

### How do I call a Code Blue - Pediatric Medical Emergency?

1. Dial **55555** (POMH staff dial 461 and call the code themselves).
2. Tell the operator you have a Code Blue - Pediatric Medical Emergency.
3. State your specific location in the hospital (department or unit); if the child is a patient, state room number and provider.
4. Code Blue - Pediatric Medical Emergency should be called on children from birth to 18 years of age.




Page 3 of 16

## Broselow™ Tape

### What is Broselow™ Tape?

- The Broselow™ tape utilizes a length-based system to help determine the approximate weight of a child, the corresponding medication dosages, and the appropriate size equipment needed for that child.
- The tape is divided into nine colored zones corresponding to different estimated weights.

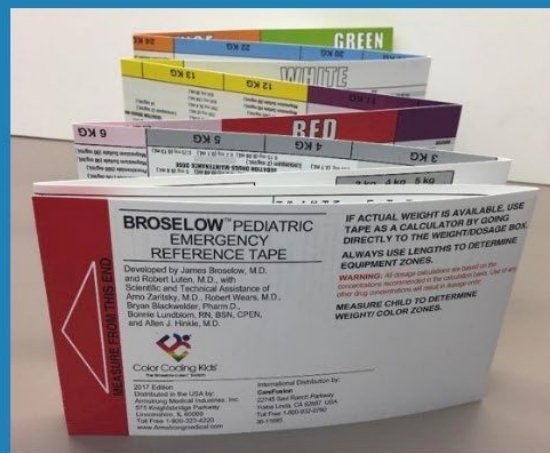

Page 4 of 16



## Using Broselow™ Tape (cont.)

- Stop your free hand at the bottom of the child's heel (not the toes). The edge of the free hand that lands on the tape adjacent to the child's heels indicates the child's approximate weight in kilograms and the child's corresponding color zone.




**\*Make sure to measure the child with his/her shoes off.\***

If the child is longer/larger than can be measured with the tape, stop and proceed as you would with an adult.

## Broselow™ Tape Location

The tape is located in the first drawer of the Broselow™ Pediatric Resuscitation Cart.

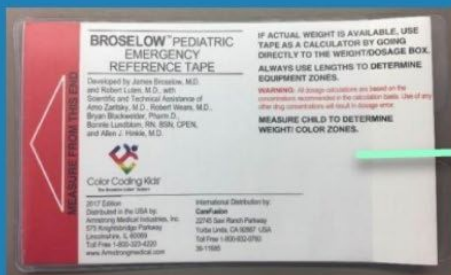

## Medication Tray

The medication tray is found in the bottom drawer of the cart. All medications in the medication tray are listed below\*:

Medication	Proposed Stock
Adenosine 6mg/2mL Vial	3
Amiodarone 450mg/9mL Vial	1
Atropine 1mg/10mL Syringe	2
Calcium Chloride 10% 10mL Syringe	1
Dextrose 10% 250 mL IVPB	1
Dextrose 5% 250 mL IVPB	1
Dextrose 5% 100 mL IVPB	1
Epinephrine 1mg/10mL Syringe	3
Epinephrine 1mg/1mL	5
Infant Dextrose 25% 2.5gm/10mL Syringe	2
Lidocaine 100mg/5mL Syringe	1
Magnesium 5 gm/10 mL Vial	1
Naloxone 2 mg/2 mL Syringe	2
Norepinephrine 4mg/4mL Vial	1
Sodium Bicarb 4.2% 2.5 mEq/5 mL Vials	6
Sodium Chloride 0.9% 500 mL IVPB	1

\* All medications are subject to shortages

\*\*Medication location may vary slightly in your cart

Page 9 of 16

## Knowledge Check 1

To call a **Code Blue Pediatric Medical Emergency** for any child between the ages of birth and 18 years of age, you would call\*

- "0" for the operator
- 55555
- 55550
- 911

\*At POMH, staff should dial 461 and page the code themselves.

Page 10 of 16

## Knowledge Check 2



When measuring with the Broselow™ Pediatric Emergency Tape, the red end of the tape is placed by the child's head.

- True
- False

## Knowledge Check 3



If the child is longer than the Broselow™ tape, what should you do?

- Estimate what weight the child is and go from there.
- Stop and proceed as you would with an adult patient.
- Weigh the patient before performing CPR.


## Knowledge Check 4



**On the Broselow™ Pediatric Resuscitation cart, where will you find the Broselow™ Pediatric Emergency Tape?**

- First drawer of the cart.
- Bottom drawer of the cart.
- On top of the cart.

## Knowledge Check 5



**On the Broselow™ Pediatric Resuscitation cart, where will you find the medication tray?**

- On top of the cart.
- First drawer of the cart.
- Bottom drawer of the cart.

## Choose Your Region Below:




**This course will now branch off to offer region-specific information. Please choose the appropriate button for the region you work in:**

**South Region  
(POMH,  
Manistee, Cadillac)**

**Central Region  
(Munson  
Medical Center)**

**East Region  
(Grayling, OMH,  
Charlevoix)**

## South Region



The rest of the course will be specific to the South Region's Broselow™ Resuscitation Carts.

## General Information



Cadillac cart



POMH cart



Manistee carts

The second through seventh drawers in the cart contain different color-coded modules based upon the length of the child as identified by the tape. The top and bottom drawers contain general supplies and equipment which can be used for any size patient.

## Cart Locations

### Cadillac:

- Emergency Department
- Inpatient Unit 3B
- PACU
- Inpatient (2nd floor) Supply Closet

### Manistee:

- Emergency Department (trauma bay)
- Surgery

### Paul Oliver Memorial Hospital (POMH):

- Emergency Department

## Where's the Defibrillator?




- Zoll Defibrillators are not always kept on Broselow™ carts.
- If needed, obtain the defibrillator from the adult crash cart nearest to the emergency location.



Page 4 of 5

## Summary

Click on each photo below to review:

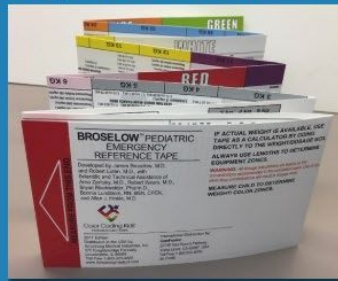

To call a pediatric code, **dial 55555** and tell the operator you have a **Code Blue - Pediatric Medical Emergency**. State your specific location in the hospital (department or unit); if the child is a patient, state room number and provider.

- Pediatric code is called for children birth to 18 years of age.
- POMH staff must call 461 and page the code themselves.

Page 5 of 5

## Summary

Click on each photo below to review:




- The Broselow™ tape utilizes a length-based system to help determine the approximate weight of a child, the corresponding medication dosages, and the appropriately-sized equipment needed for the child. The tape is divided into nine colored zones corresponding to different estimated weights.
- It is important to place the red end of the Broselow™ tape even with the top of the child's head. The heel of the child (without shoes) designates the color zone and approximate weight of the child.

Page 5 of 5

## Summary

Click on each photo below to review:

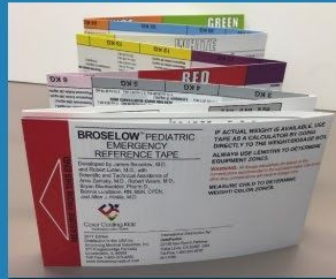

- Each drawer in the cart contains different color-coded modules based upon the length/weight of the child as identified by the Broselow™ tape.
- Pediatric resuscitation cart locations:
  - Cadillac: Emergency Department, Inpatient Unit 3B, PACU, Inpatient (2nd floor) Supply Closet
  - Manistee: Emergency Department (trauma bay), Surgery
  - POMH: Emergency Department
- Many Broselow™ carts do not contain the Zoll defibrillator and should be obtained from the nearest adult crash cart to the emergency location.

Page 5 of 5

# Munson Medical Center

The rest of the course will be specific to Munson Medical Center's Broselow™ Resuscitation Carts.

Page 1 of 19

# Broselow™ Resuscitation Cart

## General Information:

- The second through seventh drawers in the cart contain different color-coded modules based upon the length of the child as identified by the tape. The top and bottom drawers contain general supplies and equipment that can be used for any size patient.
- Pediatric resuscitation cart locations:
  - PACU
  - ED
  - B2 (Post Op area by bed 20)
  - B2 OR
  - Ground Floor PACU
  - Crash Cart Storage on C1
  - MPB
  - Interventional Radiology
  - C3



Page 2 of 19

## Top of the Broselow™ Cart

- Latex-free exam gloves (S, M, L)
- Mattress warmer
- Sharps container (attached to back rail)
- Infant resuscitation bag with mask (hangs from IV pole)
- Pediatric resuscitation bag with mask
- Neotech Snorkel suction catheter
- Yankauer suction catheter
- Crash cart return form
- Code Blue sheet and attached critique
- Clipboard with pen
- Pediatric response team call record
- Pediatric sepsis protocol folder
- Pediatric one-step CPR electrodes



Page 3 of 19

## Back of Broselow™ Cart

- Back board
- Suction canister (1200 mL)
- Suction tubing (10 ft)
- Connection tubing (3/16" x 1 1/2")



Page 4 of 19

## Left Side of Broselow™ Cart



- Oxygen tank with regulator
- Mask fluid shield
- Emergency Cardiovascular Care (ECC) book (hangs from railing)
- Outdate card

Page 5 of 19

## Right Side of Broselow™ Cart


- E-Vac portable suction (set-up)
- Wall suction regulator



Page 6 of 19

# First Drawer - Gray Drawer


Click in the rectangles to learn the items contained in that area of the gray drawer.

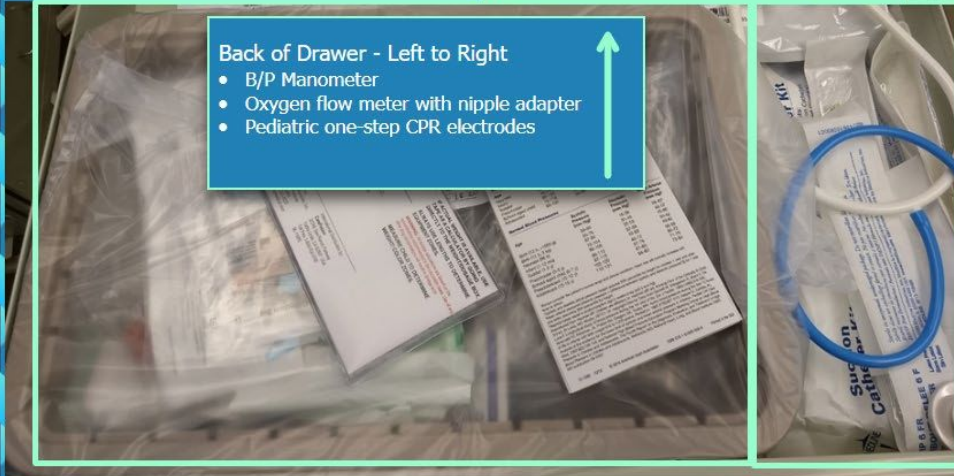

- Back of Drawer - Left to Right**
- B/P Manometer
  - Oxygen flow meter with nipple adapter
  - Pediatric one-step CPR electrodes

# First Drawer - Gray Drawer

Click in the rectangles to learn the items contained in that area of the gray drawer.

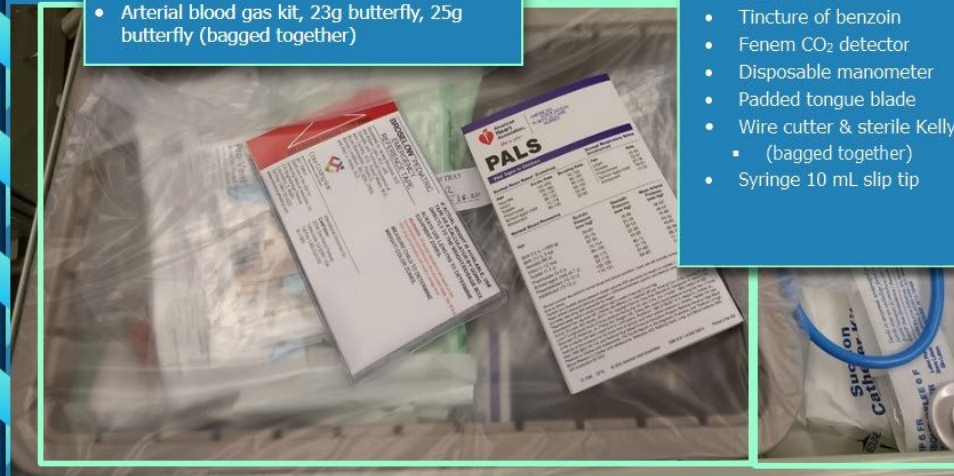


- Gray Tray**
- Miller size 0
  - Miller size 1
  - Miller size 2
  - Miller size 3
  - Macintosh size 0
  - Macintosh size 1
  - Macintosh size 2
  - Macintosh size 3
  - Magill forceps, infant
  - Magill forceps, child
  - Arterial blood gas kit, 23g butterfly, 25g butterfly (bagged together)

- Gray Tray**
- PALS pocket reference card
    - (lays on top of covered tray)
  - Pediatric Broselow™ tape
    - (lays on top of covered tray)
  - CO<sub>2</sub> mini stat detector
  - Pediatric pulse ox adhesive sensor
  - Infant pulse ox adhesive sensor
  - Tape cloth 1/2"
  - Tape cloth 1"
  - Tincture of benzoin
  - Fenem CO<sub>2</sub> detector
  - Disposable manometer
  - Padded tongue blade
  - Wire cutter & sterile Kelly forceps
    - (bagged together)
  - Syringe 10 mL slip tip

## First Drawer - Gray Drawer

Click in the rectangles to learn the items contained in that area of the gray drawer.

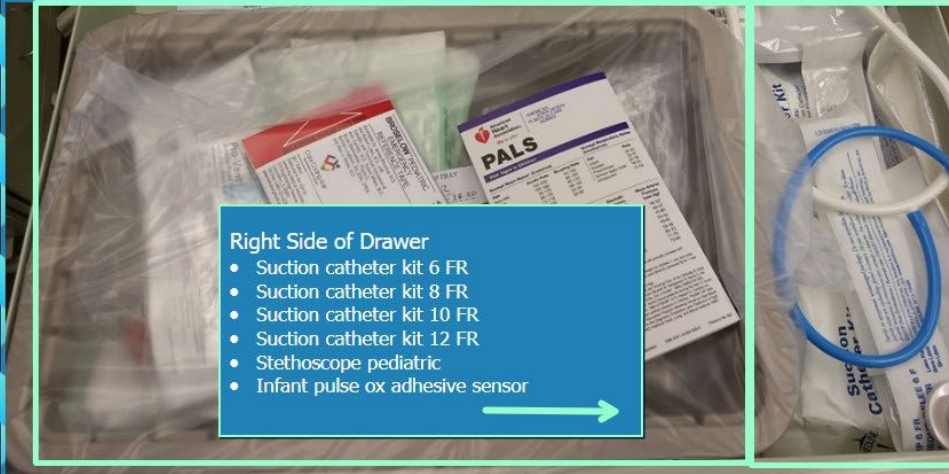

Page 7 of 19

## Color-Coded Drawers

Color-coded drawers match the zones on the Broselow™ Tape.  
Each drawer contains the appropriately-sized equipment, listed below:

- Oxygen delivery, Intubation, and IV delivery modules
- BP cuff
- Urinary catheter
- Nasopharyngeal and oral airways
- Endotracheal tubes
- Telemetry stickers
- T-connector and ETCO<sub>2</sub> airway adaptor
- IV tubing



Page 8 of 19

## Oxygen Delivery Module



Pediatric non-rebreather mask  
Oral airway




## Intubation Module



- Endotracheal tube stylet
- Endotracheal tube
- Suction catheter
- Nasogastric tube
- 36" adhesive tape
- Water soluble lubricating jelly packet
- 3" x 3" gauze pad
- Miller laryngoscope blades\*\*

\*\* **NOTE: DO NOT** use the laryngoscope blades found in the Intubation Module! **Instead,** use the laryngoscope blades found in the first gray drawer of the cart.

## IV Delivery Module

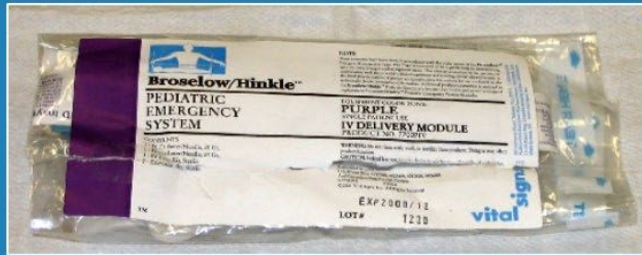

IV catheter needles  
IV prep kit, sterile  
Extension kit, sterile



Page 11 of 19

## Bottom Drawer

### Pediatric Medication and Solution Tray

Packaged on top of medication tray in zip lock bags

- Tape, adhesive 1"
- Tape, micropore 1"
- Arm board pediatric 2" x 5"
- 3-way stopcock
- Syringe 30 mL luer lock
- Needle 1" x 23 GA



Page 12 of 19

## Where's the Defibrillator?




- Zoll Defibrillators are not kept on the Broselow™ Carts.
- Remember to get the defibrillator from the adult crash cart nearest to the emergency location.



Page 13 of 19

## Summary

Click on each photo below to review:

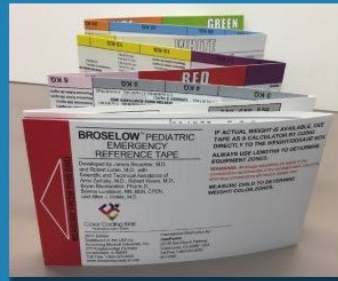

### Calling a Code:


To call a pediatric code, dial **55555** and tell the operator you have a **Code Blue - Pediatric Medical Emergency**. State your specific location in the hospital (department or unit); if the child is a patient, state room number and provider.

- Pediatric code is called for children birth to 18 years of age.
- NICU and Maternity will not call these codes overhead for inpatient infants located in these areas. If this occurs to a visitor in these areas, a Code Blue would be called.

Page 14 of 19

## Summary

Click on each photo below to review:

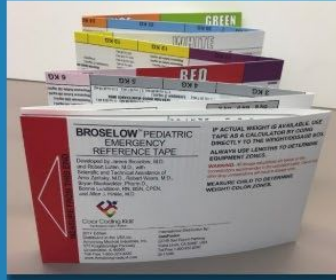


- The Broselow™ tape utilizes a length-based system to help determine the approximate weight of a child, the corresponding medication dosages, and the appropriately-sized equipment needed for the child. The tape is divided into nine colored zones corresponding to different estimated weights.
- It is important to place the red end of the Broselow™ tape even with the top of the child's head. The heel of the child (without shoes) designates the color zone and approximate weight of the child.

Page 5 of 5

## Summary

Click on each photo below to review:

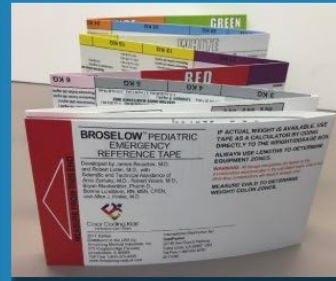

### Broselow™ Cart:

- Each drawer in the cart contains different color-coded modules based upon the length/weight of the child as identified by the Broselow™ tape.
  - Pediatric resuscitation cart locations: C3, PACU (main level and 2<sup>nd</sup> floor), OR (2<sup>nd</sup> floor), ED, MRI, Angio Lab, CPD, and MPB.
- DO NOT use the laryngoscope blades found in the Intubation Module! Instead, use the laryngoscope blades found in the first gray drawer of the cart.
- The Zoll is not on the Broselow™ cart. This should be obtained from the nearest adult crash cart to the emergency location.

Page 14 of 19

## Knowledge Check 6

On the Broselow™ Pediatric Resuscitation cart, where will you find the infant and pediatric resuscitation bag(s)?

- First drawer of the cart.
- Hanging from the IV pole.
- Bottom drawer of the cart.

## Knowledge Check 7

There is an oxygen tank supplied on each Broselow™ cart.

- True
- False

## Knowledge Check 8



When measuring with the Broselow™ Pediatric Emergency tape, the length of the child indicates which color drawer in the Broselow™ Resuscitation cart you will use.

- True
- False


## Knowledge Check 9



Each colored drawer has the appropriate color-coded intubation module with the correct equipment size for the measured child.

- True
- False

## Knowledge Check 10



Since there is no Zoll defibrillator on the Broselow™ cart, one should be obtained from the nearest adult crash cart.

- True
- False

## East Region



The rest of the course will be specific to the East Region's Broselow™ Resuscitation Carts.

## General Information



OMH cart & resuscitation pack



The second through seventh drawers in the cart contain different color-coded modules based upon the length of the child as identified by the tape. The top and bottom drawers contain general supplies and equipment which can be used for any size patient.



Grayling cart



Charlevoix cart

## Cart Locations

### Otsego:

- Emergency Department
- ICU
- Surgery - Instead of a Broselow™ Cart, there is a pediatric resuscitation pack on top of adult crash cart

### Grayling:

- Emergency Department
- Outpatient Surgery
- PACU

### Charlevoix:

- Emergency Department (Triage Room 4)
- OB Storage Room

## Where's the Defibrillator?




- Zoll Defibrillators are not always kept on Broselow™ carts.
- If needed, obtain the defibrillator from the adult crash cart nearest to the emergency location.



Page 4 of 5

## Summary

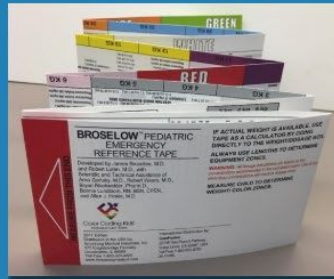

To call a pediatric code, **dial 55555** and tell the operator you have a **Code Blue - Pediatric Medical Emergency**. State your specific location in the hospital (department or unit); if the child is a patient, state room number and provider.

- Pediatric code is called for children birth to 18 years of age.

Page 5 of 5

## Summary


Click on each photo below to review:



- The Broselow™ tape utilizes a length-based system to help determine the approximate weight of a child, the corresponding medication dosages, and the appropriately-sized equipment needed for the child. The tape is divided into nine colored zones corresponding to different estimated weights.
- It is important to place the red end of the Broselow™ tape even with the top of the child's head. The heel of the child (without shoes) designates the color zone and approximate weight of the child.

Page 5 of 5

## Summary

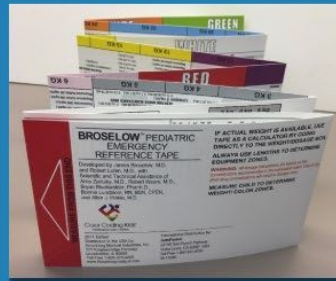

- Each drawer in the cart contains different color-coded modules based upon the length/weight of the child as identified by the Broselow™ tape.
- Pediatric resuscitation cart locations:
  - Otsego: Emergency Department, ICU, Surgery - Instead of a Broselow™ Cart, there is a pediatric resuscitation pack on top of adult crash cart
  - Grayling: Emergency Department, Outpatient Surgery, PACU
  - Charlevoix: Emergency Department (Triage Room 4), OB Storage Room
- Many Broselow™ carts do not contain the Zoll defibrillator and should be obtained from the nearest adult crash cart to the emergency location.

Page 5 of 5

## References

- Munson Medical Center Policies and Procedures. (2025, May 9). *Code Crash Carts for Adult, Pediatric (Broselow™), and Infant Drugs/ Supplies Exchange Procedure*. PolicyStat.
- Munson Medical Center Policies and Procedures. (2025, June 5). *Pediatric Response Team Protocol for Pediatric Patients*. PolicyStat.
- Vital Signs Inc. *Broselow™ Pediatric Emergency Tape*. (2019). Ed., A. Armstrong Medical Industries, Inc.



Origination 12/13/2023  
Last 6/3/2025  
Approved  
Effective 6/3/2025  
Last Revised 6/3/2025  
Next Review 6/2/2028

Owner Jennifer Standfest: CNO  
Area/Department Nursing  
Applicability MMC, Cadillac, Charlevoix, Grayling, Otsego

## Cardiac Telemetry Monitoring

### Purpose

To enhance patient safety and clinical consistency by outlining continuous cardiac monitoring guidelines, arrhythmia detections and overall alarm management.

### Definitions

1. **Cardiac Monitoring/Telemetry Monitoring:** Continuous cardiac rhythm display at the bedside and/or transmitted to a central monitoring console that can provide alarms or print/save rhythm strips.
2. **Telemetry Technician:** Licensed or unlicensed staff member with training and competency in electrocardiogram (ECG) rhythm interpretation.
3. **Telemetry Observer:** An individual assigned to listen for and/or observe specific visual cues with the intention of escalating information to a resource trained to assess and/or intervene in a specific situation.

### Policy

- A. An order is needed to initiate and discontinue cardiac monitoring. Orders should specify any parameters and any circumstances in which the patient can be temporarily or permanently removed from monitoring.
- B. When initiating cardiac monitoring, the following identifiers are used:
  1. 10-digit account number
  2. Last Name, First Name (NOTE: This will automatically pull through ADT feed if 10-digit account number is entered correctly)

- C. The Registered Nurse (RN) is responsible to:
1. Initiate and maintain continuous monitoring and to perform initial review and adjustment of settings and alarm parameters.
  2. Regularly review and interpret cardiac rhythm and document findings in the chart.
  3. Assess need for continued cardiac monitoring daily, using provider orders or protocol, where applicable.
  4. Report clinically relevant abnormalities identified on review or by alarm/event review to the provider. Abnormalities include but are not limited to:
    - a. Any new dysrhythmia (i.e., tachy or brady arrhythmia exceeding alarm)
    - b. Heart block
    - c. New atrial fibrillation or flutter or inadequate rate control of these rhythms
    - d. Ventricular tachycardia/fibrillation
    - e. Supra-ventricular tachycardia
    - f. Any symptomatic patient with a dysrhythmia
    - g. Any dysrhythmia requiring immediate treatment
  5. Initiate code response or other facility specific rapid response protocols or appropriate emergency interventions
  6. The RN may delegate tasks to appropriately trained support personnel. These may include, but are not limited to: equipment preparation, skin preparation, electrode application/reapplication, application of monitoring equipment.
- D. Where present, telemetry technicians may review and adjust specific settings and alarm parameters and may interpret cardiac rhythms, complete specific documentation, and shall report abnormalities to the RN.
1. The technician will monitor each telemetry unit for ventricular tachycardia, ventricular fibrillation, asystole, tachycardia and bradycardia, low battery and lack of rhythm. The telemetry technician will contact the nurse with findings.
  2. A telemetry log may be kept on each unit with pertinent info such as the patient's name, dominant rhythm, assigned nurse and the direct phone number(s) for the assigned care team.
- E. A telemetry technician and/or any RN not directly responsible for the patient's care who observes events or responds to alarms at the bedside or central monitoring station will notify the primary nurse of any changes in the patient's condition, monitor settings, or alarm parameters.
- F. Where present, telemetry observers are identified 24 hours a day. The telemetry observer may perform other clerical duties that do not remove them from direct view or audio of the monitor. The observer will arrange for another trained observer or nurse to fill the role temporarily if needed for breaks or to perform other job duties away from the area.
- G. Any support personnel should consult with/notify the appropriate individual (eg., telemetry observer or technician, RN, etc.) prior to removing a patient from monitoring for showering,

procedures/testing or discharge.

## Electrode and Lead Placement, Battery Replacement

- A. Electrodes are applied according to Lippincott Procedures - Cardiac monitoring (lww.com) instructions found online. Electrodes shall be changed daily and as needed (PRN) or in accordance with manufacturer recommendations.
- B. Lead placement should be confirmed at the beginning of each shift, along with verification the monitor / transmitter is functioning properly and that suitable battery life remains.
- C. Battery change should occur minimally when "low battery" signal appears, or with approximately 25% battery life remaining.

## Lead Selection

- A. Lead II is generally selected as the standard monitoring lead.
- B. For a standard 5 lead system, V1 is commonly selected as the second lead. An alternate lead may be selected based on which provides a clearer trace, more prominent or upright waves, or by which a particular area of the heart can be better monitored.

## Cleaning

- A. Upon discontinuation of telemetry monitoring, the telemetry unit and electrodes are cleaned per manufacturer instructions.

## Cardiac Rhythm Waveforms and Documentation

- A. A rhythm strip will be measured, interpreted, and documented per the following guidelines:
  - 1. Rhythm interpretation is ongoing and documented as part of the nursing assessment
  - 2. Inpatient care (critical, intermediate, or telemetry care departments) at admission, each shift with initial RN assessment, and with any significant change in rhythm or significant symptoms
  - 3. Emergency Department (ED) at admission and with any life-threatening rhythms or significant changes in patient condition
  - 4. Rhythm waveform documentation should include the name of identified rhythm, heart rate, PR/QRS/QT intervals where applicable, and the name of the RN or Telemetry Technician performing the documentation.

## Monitoring Guidelines

- A. HR alarms will be set appropriately to the patient's baseline HR, rhythm, clinical condition or treatment plan by an RN or Telemetry Technician.
- B. If a monitored patient has a pacemaker, the pacemaker detection function of the cardiac monitor must be turned ON

Refer to Munson Healthcare (MHC) entity specific intravenous (IV) Medication Guidelines and/or consult with pharmacy for information related to risk of prolonged QT interval and for IV medication administration and required monitoring.

- C. QT interval monitoring functions of the cardiac monitors may be utilized by the RN/Tele Tech as an adjunct to patient / rhythm assessment. A patient with a baseline prolonged QT or on a medication that has the potential of prolonging the QT interval may have orders for more frequent QT measurements.
- D. ST segment monitoring and ST mapping functions of the cardiac monitors may be utilized by the RN/Tele Tech as an adjunct to patient assessment. (Note: some clinical conditions make it difficult to achieve accurate ST monitoring i.e., atrial fib or flutter with an irregular baseline, ventricular pacing, left bundle branch block. Consider turning ST monitoring off in these conditions).
- E. Silencing Alarms:
  - 1. A trained telemetry observer or technician or a registered nurse may silence clearly erratic/false alarms such as those caused by motion or artifact while requesting evaluation by clinical personnel.
  - 2. A lethal rhythm alarm may be silenced by a Telemetry Technician or RN after the RN evaluates the rhythm and/or patient condition.

## Alarm Settings and Clinical Management

- A. The Clinical Engineering department has oversight for the testing and maintenance of clinical devices to ensure accurate settings, proper operation, and detectability of alarms.
- B. Monitor settings are configured according to manufacturer recommendations to enhance patient safety. A copy of all configuration settings is maintained by the Clinical Engineering department. These settings may only be changed with approval of the Cardiac Monitoring Steering Committee or the Cardiac Monitoring Alarm Committee, with the endorsement of the Clinical Leadership Council.
- C. Arrhythmia monitoring will be on and audible for all monitored patients, with the exception of patients who are receiving end of life care, where death is anticipated and an order for comfort care is present.
- D. Alarm volume should be set audibly so that nursing staff is able to hear and respond appropriately to non-critical and critical alarms. It is the responsibility of the bedside nurses, the unit coordinator, and other clinical staff to maintain the appropriate alarm volume which decreases noise pollution for patients and visitors, while ensuring prompt staff notification of alarm situations.
- E. Select alarm parameters are unlocked and able to be adjusted on an individual basis by the RN, Telemetry Technician, or other licensed clinician within their scope of service.
- F. All monitor alarm settings should be adjusted to reflect patient or condition specific values and should be reviewed and adjusted (if indicated) at admission, each shift, and as needed by the RN and/or Telemetry Technician.
  - 1. The nursing staff member will determine the appropriate response to the alarm; however, the nurse is responsible to confirm findings, verify patterns, and evaluate

interpretations through patient assessment. The response to an alarm may include but is not limited to silencing the alarm, recording the strip, and/or initiating emergency interventions.

2. In the event of a Code Blue or Cardioversion, an event strip will be documented containing the initiation of the event and documentation of changes in rhythm continuing through termination of efforts. As an alternative, a strip from the defibrillator may be used to record the events of the Code Blue.

G. Patient care staff are familiar with alarm settings, policies and procedures.

## Transfer/Discharge Procedure

- A. At the time of transfer/discharge, the patient MUST be discharged from the bedside and/or central monitoring console, and when applicable, have their encounter be dissociated from the electronic health record (EHR).
- B. Refer to manufacturer instructions for use for specific steps to transfer or discharge patient.

## Transport Monitoring

- A. An RN (or in some cases, a paramedic) shall accompany the patient for transport if the patient is in critical condition, hemodynamically unstable and/or on continuous vasoactive infusions.
- B. Other monitored patients transported by unlicensed staff will be monitored remotely by the telemetry technician, telemetry observer, or RN. A portable phone will be assigned and in the possession of the staff member closest to/responsible for the patient at all times. Monitoring staff will use this phone to communicate emergency conditions and request immediate assistance for the patient.

## Reference

1. Wiegand, D. L. (Ed.). (2017). AACN Procedure Manual for High Acuity, Progressive, and Critical Care (7th ed., pp. 467-476). St. Louis, MO: Elsevier.

## Keywords

*Cardiac, Telemetry, Monitoring, Tele Tech*

## Approval Signatures

Step Description	Approver	Date
System Policy Oversight Committee	Terri Fries: Document Mgmt Spec	6/3/2025
CNO Council	Jennifer Standfest: CNO [AM]	6/2/2025

## Applicability

Cadillac Hospital, Charlevoix Hospital, Grayling Hospital, Munson Medical Center, Otsego Memorial Hospital

## Standards

No standards are associated with this document

COPY

Status **Active** PolicyStat ID **15460185**



Origination 12/18/2009  
Last Approved 11/7/2025  
Effective 11/7/2025  
Last Revised 11/7/2025  
Next Review 11/6/2028

Owner Brendan Franklin:  
Dir Nursing  
Critical Care &  
Stroke  
Area/  
Department Nursing  
Applicability MMC  
Tags Policy

## Critical Care Standards

### Purpose

To provide a standard for nursing care in the critical care patient population and enhance coordination of care among the healthcare team.

### Scope

Critically ill patients receiving care in A2, A3, and the Intensive Care Unit (ICU).

### Policy

- A. All Registered Nurses (RN) are prepared to:
  - 1. Utilize corresponding policies and procedures to implement nursing process for patient care.
  - 2. Respond to urgent and emergent situations.
  - 3. Perform specialized nursing procedures specific to critically ill patient needs.
  - 4. Administer care and specialized interventions in the critically ill patient population.
  - 5. Document care and specialized interventions.
- B. Nursing care of critically ill patients in critical care units includes:
  - 1. Systems Assessments:
    - a. Perform and document head-to-toe assessment every 4 hours, unless the patient's condition or physician order indicates alternative frequency.
    - b. Including the following:

- i. Recent and relevant events and patient outcomes.
- ii. Device use, care and management and patient tolerance.
- iii. Wound/skin care and management.
- iv. Pain assessment and documentation unless patient condition requires a greater frequency. Pain reassessment will occur after treatment (per the [Pain Management](#) policy).
- v. All individualized care needs for the critically ill patient.

2. Lines/Tubes/Devices

- a. Assessment is completed and documented every four hours including type, station, and status.

3. Vital signs:

- a. Blood pressure, heart rate, respiratory rate, and pulse oximetry with oxygen delivery method are monitored and recorded hourly, unless otherwise ordered or the patient's condition indicates alternative frequency.
- b. When titrating medications, vital signs are documented according to medication order titration guidelines.
- c. Temperatures are recorded at a minimum of every 4 hours unless otherwise ordered or the patient's condition indicates alternative frequency. Temperatures are recorded hourly when warming or cooling measures are used.
  - i. All patients with abnormal temperatures are assessed for potential complications related to hypothermia or hyperthermia.
  - ii. RN may initiate warm blankets, commercial warming devices, and/or fluid warmer on any patient with a rectal or core temperature of less than 35.6°C. Provider must be notified.
  - iii. RN may initiate cooling blankets on any patient with a rectal or core temperature of greater than 38°C if antipyretics and other means of external cooling have been ineffective. Provider must be notified.
  - iv. The fluid warmer may be used for any patient with a rectal or core temperature of less than 35.6°C.

4. Hemodynamic monitoring:

- a. Electrocardiogram (ECG) monitoring is established upon arrival and maintained throughout hospitalization.
- b. Invasive line pressures are documented every hour unless otherwise ordered or the patient's condition indicates alternative frequency. This includes but is not limited to: arterial blood pressure (ABP), central venous pressure (CVP), pulmonary artery pressure (PAP), pulmonary capillary wedge pressure (PCWP), Intracranial pressure (ICP), cerebral perfusion pressure (CPP).

- c. Arterial lines and pulmonary artery catheters must always be transduced. Exception: during magnetic resonance imaging (MRI) testing.
  - d. Transport monitoring: Minimum transport monitoring of critical care patients will include continuous ECG, blood pressure, and oxygen saturation monitoring. Arterial lines and pulmonary artery catheters must always be transduced, even during transport. Additional monitoring may be held or continued during transport.
5. Respiratory:
- a. Airway or endotracheal tube (ETT) station is documented every four hours.
  - b. ETT is repositioned every four hours and prn in collaboration with Respiratory Therapy (RT).
  - c. An RN may extubate a patient upon a physician's order or per protocol, with RT at the bedside.
6. Fluid volume status and intake & output (I&O):
- a. Patients require strict hourly I&O with daily weights unless otherwise ordered or the patient's condition indicates alternative frequency.
7. Nutrition:
- a. The goal is to start nutrition within 24 hours of admission, based on patient condition. Diet/nutrition is monitored daily, including type of nutrition, source and patient tolerance. RN may initiate dietary consult as needed.

Document ID: 070.065

## Approval Signatures

Step Description	Approver	Date
System Policy Oversight Committee	Terri Fries: Document Mgmt Spec	11/7/2025
CNO	Tamara Putney: VP and CNO Patient Care Services	11/7/2025
Mgr Nursing Services	Amber Bowers: Mgr Nursing Services	11/5/2025
Document Owner	Brendan Franklin: Dir Nursing Critical Care & Stroke	11/5/2025

---

## Applicability

Munson Medical Center

## Standards

No standards are associated with this document

COPY

# Fire Safety in Anesthetizing/ Procedural Areas

Jeannette Reynolds, MSN, BBA, RN, CPAN

Kathy Sahs, BS, CHSP

Sam Smith, MSN, RN, CCRN, SANE

Magdalena Stewart, DNP, CNS

Pat Wyers, BSN, RN, CNOR

July 2024

back

exit

next

# Goal and Objectives

## Goal:

To educate anesthetizing/procedural area staff about the recommended actions for fire prevention and fire response.

## Objectives:

After completing this activity, the participant will be able to:

1. Identify the three components of the fire triangle.
2. Identify steps for fire prevention interventions.
3. Describe the staff's role in fire safety.
4. Discuss the steps to extinguish a fire.



# Procedural Fire Facts

According to The Joint Commission (TJC)

- 90-100 surgical fires occur yearly.
- 70% involve use of an electrosurgical device (ESU), also known as a Bovie.
- 15% are related to use of a light source.
- Other contributing factors include:
  - Inadequate orientation, understanding and/or communication of fire risk in procedural areas
  - Insufficient time-out procedures
  - Overconfidence, distraction, or loss of situational awareness
  - Equipment malfunction



back

exit

next

## It Happens Here!

In the first quarter of 2022, an MHC OR had two fire/unintentional smoke events from equipment (laser and surgical drill). No patient or staff injury occurred.

Also in April 2022, a fire occurred when a patient applied petroleum jelly to their lips while on high-flow oxygen. The patient sustained first- and second-degree burns.



Page n of nn



# Fire Triangle

There are three elements necessary for a fire:

- Ignition source
- Fuel
- Oxidizer



# Common Ignition Sources

An ignition source is anything providing enough energy to start a fire:

- ESU/Bovie
- Argon beam coagulator
- Power tools (e.g., drills, burrs)
- Laser
- Fiber Optic light cords
- Defibrillator
- Electrical equipment



back


exit

next

# Common Fuels

A fuel is anything that will burn:

- Alcohol-based skin antiseptic agents (preps)
- Drapes
- Gowns
- Endotracheal tubes
- Skin degreasers/tinctures/aerosols
- Body tissues and hair
- Intestinal gases
- Petroleum-based products

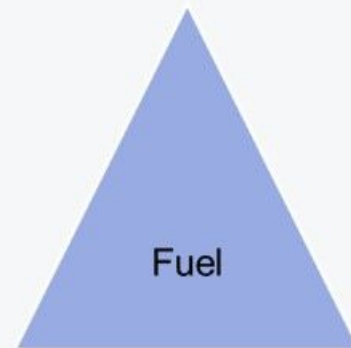

Page n of nn



back


exit

next

# Common Oxidizers

An oxidizer is a gas which supports combustion:

- Oxygen
- Nitrous oxide

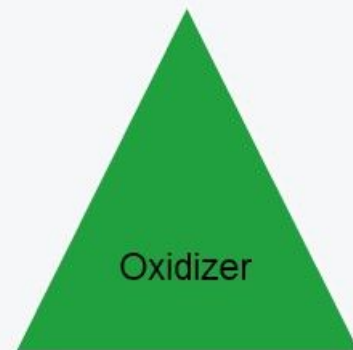

back

exit

next

# Fire Risk Assessment

Fire risk assessment is a team effort.

As part of the preprocedural briefing process, the proecdural team should initiate a fire risk assessment to assess for the presence of the three elements of the fire triangle (AORN).

Page n of nn



[back](#)[exit](#)[next](#)

## Fire Risk Assessment *(cont.)*

Before each procedure, evaluate the following:

- Are there alcohol-based prep agents or other flammable solutions being used?
- Is the procedure being performed above the xiphoid process?
- Is there open oxygen or nitrous oxide being administered?
- Is an ESU, laser, fiber-optic light cord, defibrillator, drill, or saw being used?
- Are there other possible contributors?



You must complete the activity.

# Controlling Ignition Sources

Click each arrow:



## Fiber-Optic Light Source:

- Place the light source in standby mode or turn it off when not in use.
- Inspect light cables before use. Remove from service if broken light bundles are visible.
- Place the scope and light source on a designated heat-resistant surface when not in use.



[back](#)[exit](#)[next](#)

# Controlling Fuels

## Surgical Skin Prep:

- Prevent pooling of skin prep solutions.
- Remove and discard prep-soaked materials, ensuring they are at least 3 feet from an ignition source.
- Skin prep dry time should follow manufacturer instructions for use to allow fumes to dissipate before draping.
- Allow chemicals to dry (e.g., alcohol, collodion, tinctures).
- Use water-soluble gel to cover facial hair.



[back](#)[exit](#)[next](#)

# Controlling Oxidizers

Considerations for oxygen/flammable gas administration:

- Check the anesthesia circuits for possible leaks prior to the start of the procedure.
- Tent the surgical drapes to allow for free air flow.
- Keep the oxygen percentage as low as possible on non-intubated patients.
- Inform the surgeon when an open oxygen source is being used.
- Turn off oxygen or nitrous for 1 minute prior to use of an ignition source in head, neck, or upper chest procedures.

Page n of nn



back

exit

next

## Controlling Oxidizers *(cont.)*

### Oropharynx Procedures

- Inflate the endotracheal tube cuff with tinted saline.
- Evacuate intended surgical smoke from small or enclosed spaces.
- Pack wet sponges around the back of the patient's throat.
- Document placement and removal of throat sponges.
- If oxygen is being used, suction the patient's oropharynx deeply before using the ignition source.

Page n of nn



back

exit

next

## See Unintended Smoke or Flames?

Pull the fire alarm!

All team members should be alerted to the presence of a fire or unintended smoke, no matter how small. Alerting other team members decreases the risk of injury to the patient and personnel.



Page n of nn





back

exit

next

## Fire Pull Station Locations and Responders

- It is the responsibility of each team member to be aware of the locations for fire pulls in his/her areas.
- When a fire pull is activated, the facility response team and the fire department will respond to the alarm.
- Assign a staff member to assist responders with donning disposable coveralls and lead them to the location of the fire.

Page n of nn



back

exit

next

# Code Red Fire Response

Remember the acronym **RACE**:

**R Rescue** anyone in immediate danger.

**A Alarm** - activate nearest fire alarm.

Immediately notify the Main Desk/Unit Charge.

**C Contain** the fire to prevent it from spreading (close doors).

**E Extinguish** the fire using appropriate devices. **Evacuate**, if required.

Page n of nn



back

exit

next

## Medical Gas Shut-off

Be aware of the medical gas shut-off valve locations in your area. They are typically located outside the procedural suite and labeled.

In the event of a fire, the team should critically evaluate medical gas shut off for that specific area, then communicate medical gases have been emergently shut off in your location.

The decision to further shut off medical gases is made upon mutual consent among Nursing Administration, Respiratory Therapy, Facilities services, and anesthesia providers (if present).



back

exit

next

## Extinguish a Fire Using Solution

- Douse the base of the fire with a nonflammable liquid (saline or water) if readily available.
- Impermeable drapes must be removed to effectively extinguish the fire.



Page n of nn



back

exit

next

## Extinguish a Fire by Smothering

- Keep your body away from fire.
- Hold towel between fire and patient's airway.
- Drop the end of towel closest to the head.
- Drop the other end of towel over the fire.
- Sweep hand over towel from head toward feet. **DO NOT PAT** the fire! This fans the flames and expands the fire.
- Lift the towel carefully to determine if flames are extinguished.
- Remove drapes or burned material from patient and inspect for injury.



Page n of nn



# Extinguish a Fire Using a Fire Extinguisher

Remember the acronym **PASS**:

**P** Pull the pin.

**A** Aim nozzle at the base of the fire.

**S** Squeeze the handle to release the extinguishing agent.

**S** Sweep the stream over the base of the fire.

If possible, spray extinguisher away from the patient or other people.



<http://www.dol.gov>



# Fire Extinguisher Types

Most patient care areas have ABC multipurpose fire extinguishers available for use.

- A. Fires involving wood, paper, cloth, and most plastics.
- B. Fires involving flammable liquids or grease.
- C. Fires involving energized electric equipment.

Some areas (OR, Sterile Processing, and MRI suites) may also have specialty extinguishers such as BC, CO<sub>2</sub>, or water mist (non-magnetic) available for use.



back

exit

next

# Airway Fire Management

Assist the anesthesia provider to:

1. Stop the medical gas flow.
2. Disconnect the breathing circuit.
3. Pour normal saline or water directly into the airway, if directed.
4. Remove the endotracheal tube, saving any burned segments.
5. Examine the airway.
6. Re-establish airway support.

Page n of nn





back

exit

next

## After a Fire is Extinguished

1. Inspect the area for a secondary fire on the underlying drapes or towels.
2. Assess the patient for injury.
3. Determine what needs to be done to complete the case (new room, tear down, supplies, instruments, etc.).
4. Complete an incident report using VOICE.
5. Notify nursing administration and the administrator on call.
6. Save all materials from the fire for inspection by facility specialists and the fire department.

Page n of nn





back

exit

next

# Fire Evacuation

Depending on the severity of the fire, evacuation may be limited to the immediate area followed by partial or total department evacuation.

Unless the patient and staff are in immediate danger, the decision to evacuate and the safest route to go occurs in conjunction with unit/facility leadership.

Page n of nn



You must complete the activity.

# Types of Evacuation

All patients and staff must be accounted for during an evacuation.  
Click each button for evacuation definitions.

## Vertical

Patients and staff are moved two floors below the fire area.  
The entire building is evacuated.

back

exit

next

# Evacuation Routes

During an emergency evacuation, follow the evacuation route/ area posted in your facility-specific policies.

Page n of nn



# Teamwork

Fire prevention and fire control takes a **critically-thinking team**.  
Keep in mind the following:

- Location of the fire alarms, extinguishers, and gas shut-offs.
- Closest evacuation route.
- Cases that are at risk for fires.
- Steps to take to prevent fires.
- Steps to take when there is a fire.
- Who to contact STAT.



back

exit

# References

Association of PeriOperative Registered Nurses Guidelines for Perioperative Practice. (2022). *Environment of Care*  
<http://online.statref.com/document/zCT1HcgrG7DjzPC-uTPnBj>

Association of PeriOperative Registered Nurses. (2022). *Fire safety toolkit*.  
<https://test.aorn.org/guidelines/clinical-resources/tool-kits/fire-safety-tool-kit>

MHC PolicyStat Evacuation Plan

MHC PolicyStat Munson Medical Center Fire Plan

MHC PolicyStat Operating Room Fire Plan

Pfander, Valerie (2017-2022). Fire Safety in the Operating Room. Munson Medical Center

Page n of nn




LEVEL 1<sup>®</sup>

# OPERATOR'S MANUAL

en

## HOTLINE<sup>®</sup> Blood and Fluid Warmer

REF HL-90

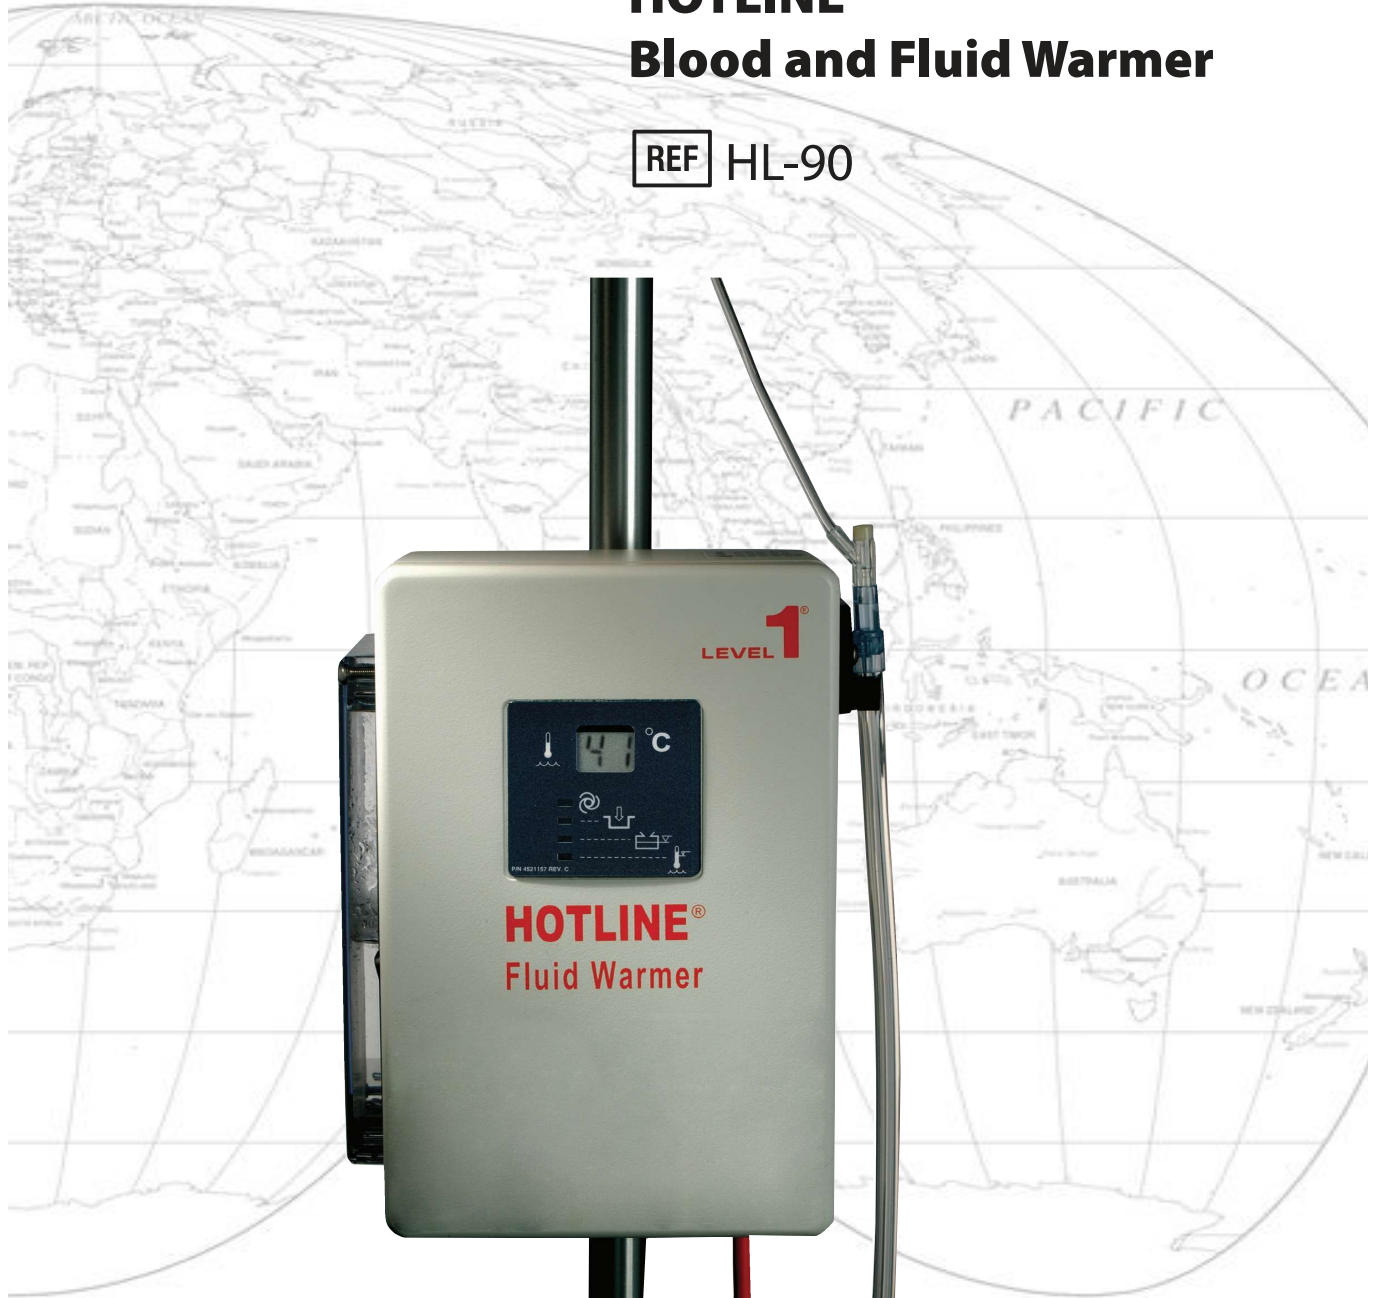

smiths medical

Page intentionally blank



**HOTLINE®**  
**Blood and Fluid Warmer**

**REF** HL-90`

**OPERATOR'S MANUAL**

PN 10011022-003

**smiths medical**

## **HOTLINE® Blood and Fluid Warmer**

Part Number: 10011022-003

This revision supercedes all previous revisions.

Every effort has been made to ensure that the information in this manual is accurate and details provided are correct at the time of printing. The company, however, reserves the right to improve the equipment shown. Mention of third-party products is for informational purposes only and constitutes neither an endorsement nor a recommendation. Smiths Medical ASD, Inc. ("Smiths Medical") assumes no responsibility with regard to the performance or use of these products.

Smiths Medical and Level 1 design marks and Level 1 and HOTLINE are trademarks of Smiths Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark office and certain other countries.

All other names and marks mentioned are the trade names, trademarks, or service marks of the respective owners.

For further information, please call your local Smiths Medical distributor or Smiths Medical direct at 1 800 258 5361 or +1 614 210 7300.

©2014, 2017, 2019, 2020 Smiths Medical.

All rights reserved.

---

# Contents

1	About this Manual	1
	<b>Indications for Use</b>	1
	<b>Conventions Used in this Manual</b>	1
2	Description	2
	<b>Components</b>	2
	<b>HOTLINE® Fluid Warming Set</b>	4
3	Important Safety Information	5
	<b>Additional WARNINGS and CAUTIONS for Accessories</b>	9
4	Assembly Instructions	10
	<b>Step 1 - Unpack the HOTLINE® Warmer</b>	10
	<b>Step 2 - Clamp the HOTLINE® Warmer to the I.V. Pole</b>	10
	<b>Step 3 - Disinfect the Reservoir</b>	11
	<b>Step 4 - Fill the Reservoir With Recirculating Solution</b>	12
	<b>Step 5 - Perform the Electrical Safety Tests</b>	12
5	Principle of Operation	13
	<b>Infusate Delivery Temperatures</b>	13
6	Operation	14
	<b>Controls and Displays</b>	14
	Display Panel	14
	Power and Alarm Test Panel	15
	Reservoir Level Display	15
	<b>Modes of Operation</b>	16
	OFF Mode	16
	ON/Operating Mode	16
	Check Disposables Mode	16
	Add Recirculating Solution Mode	17
	Over Temperature Alarm Mode	17
7	Operating Instructions	18
	<b>Step 1 - Set Up the HOTLINE® Warmer</b>	18
	<b>Step 2 - Set Up the HOTLINE® Fluid Warming Set</b>	19
	<b>Step 3 - Connect the Intravenous Administration Set</b>	20
	<b>Step 4 - Using the HOTLINE® Warmer</b>	20
	<b>Step 5 - After Use</b>	21
	Storage	21
8	Troubleshooting	22
9	Testing	24
	<b>Alarm Signal Test</b>	24
	<b>Over Temperature Alarm Test</b>	25
	<b>Add Recirculating Solution Test</b>	25
	<b>Check Disposables Test</b>	26
	<b>Temperature Verification of the Recirculating Solution</b>	26
	<b>Periodic Electrical Testing</b>	28
	Leakage Current	28
	Ground Bond Test	28

---

10	<b>Maintenance</b>	29
	<b>Maintenance Performed with Every Use</b>	29
	Clean the Exterior	29
	General Inspection	31
	<b>Disinfect the Reservoir and Change the Recirculating Solution</b>	31
	Disinfect the Reservoir	31
	Add Recirculating Solution	32
	<b>Maintenance Performed Every 30 Days</b>	32
	Disinfect the Reservoir and Change Recirculating Solution for Distilled Water and 35% Isopropyl Alcohol Solution	32
	Lubricate O-Ring Seals	32
	<b>Maintenance Performed Every 12 Months</b>	33
	Disinfect the Reservoir and Change Recirculating Solution for 0.3% Hydrogen Peroxide Solution	33
	Replace O-Rings (O-Ring Kit: P/N 80-04-001)	33
	<b>Testing HOTLINE® Warmer Operation</b>	33
	Maintenance Log	34
11	<b>Limited Warranty</b>	35
12	<b>Service</b>	37
	<b>Non-Warranty Work</b>	37
	<b>Additional Documentation</b>	37
	<b>Disposal Information</b>	38
	<b>Service Contacts</b>	38
	USA/Canada	38
	European Representative	38
13	<b>Specifications and Accessories</b>	39
	<b>System Specifications</b>	39
	<b>Electromagnetic Compliance</b>	41
	<b>Electromagnetic Environmental Recommendations</b>	44
	<b>Accessories</b>	44
14	<b>Symbols</b>	45
15	<b>Index</b>	48

## SECTION 1

# About this Manual

This operator's manual describes the assembly, use, and maintenance of the HOTLINE® Blood and Fluid Warmer. This manual is intended for use by individuals trained in the healthcare and biomedical professions.

**WARNING:** These instructions contain important information for safe use of the product. Read the entire contents of this operator's manual, including Warnings and Cautions, before using this product. Failure to properly follow warnings, cautions, and instructions could result in death or serious injury to the patient.

## Indications for Use

The HOTLINE® Blood and Fluid Warmer is designed for use with the HOTLINE® Fluid Warming Set to warm blood and intravenous (I.V.) fluids and deliver them to the patient's intravenous access site at normothermic temperatures under gravity flow conditions. The HOTLINE® Warmer is intended for use by trained medical personnel to provide routine flow of warmed I.V. fluid.

## Conventions Used in this Manual

- The HOTLINE® Blood and Fluid Warmer will be referred to as the HOTLINE® Warmer.
- The L Series Fluid Warming Sets (L-70, L-70NI, L-80) will be referred to as the HOTLINE® Fluid Warming Set or Disposable Set.

Convention	Description
<b>CONTRAINDICATION</b>	A Contraindication statement alerts the operator to conditions when the device should not be used.
<b>CAUTION</b>	A Caution statement alerts the operator to conditions that may cause malfunction, failure, or damage to the device.
<b>WARNING</b>	A Warning statement alerts the operator to conditions that may cause death or serious injury to the patient or operator.

## SECTION 2

# Description

The HOTLINE® Warmer delivers blood and intravenous fluid at normothermic temperatures by surrounding the sterile intravenous line with a layer of warmed recirculating solution. An onboard recirculating solution supply is heated to  $41.5^{\circ}\text{C} \pm 0.5$  and circulated through the outer lumen of the HOTLINE® Fluid Warming Set, which surrounds the intravenous line.

The HOTLINE® Warmer employs a safe, recirculating solution heating system, inherently free of “hot spots,” to actively warm the patient line. Electronic circuitry continuously monitors the recirculating solution temperature. The primary temperature control circuit limits the recirculating solution to  $42^{\circ}\text{C}$  maximum. In the unlikely event of a malfunction of this circuit, a second “watchdog” circuit will visually and audibly alarm and stop the recirculating solution pump if the temperature reaches  $43.1^{\circ}\text{C}$ . Fluid in the HOTLINE® Fluid Warming Set is never exposed to any damaging or dangerous temperatures while the HOTLINE® Warmer is operating.


The recirculating solution temperature and visual alarms are indicated on the Display Panel on the front of the HOTLINE® Warmer. A green Operating light illuminates on this panel when the HOTLINE® Warmer is set up and operating correctly.


## Components

The HOTLINE® components are called-out in the following series of figures.


### Front View

- 1 Socket for HOTLINE® Fluid Warming Set with the reflux plug in place
- 2 Display Panel

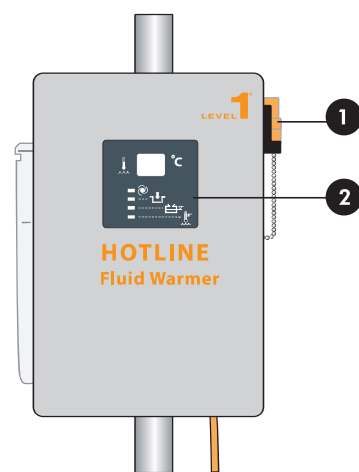


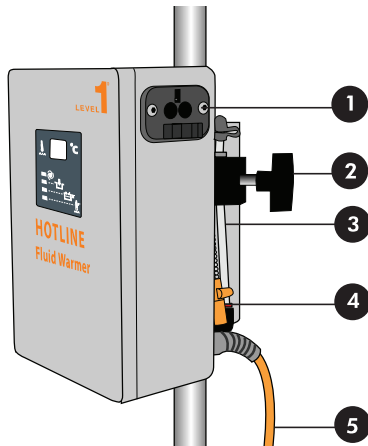**Right Side View**

- 1 Socket with the reflux plug removed
- 2 Clamp for I.V. pole
- 3 Drain tube in tube holder
- 4 Reflux plug
- 5 Power cord

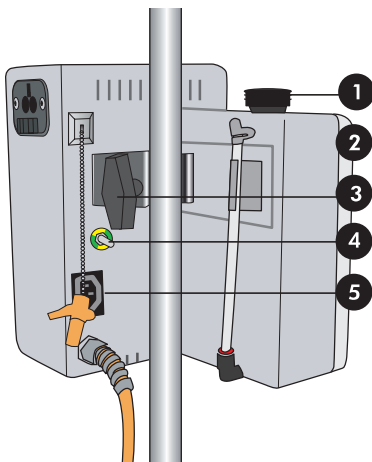**Rear View**

- 1 Fill-port plug
- 2 Drain tube in tube holder
- 3 Clamp for I.V. pole
- 4 Protective earth terminal
- 5 Auxiliary electrical outlet (uncovered)

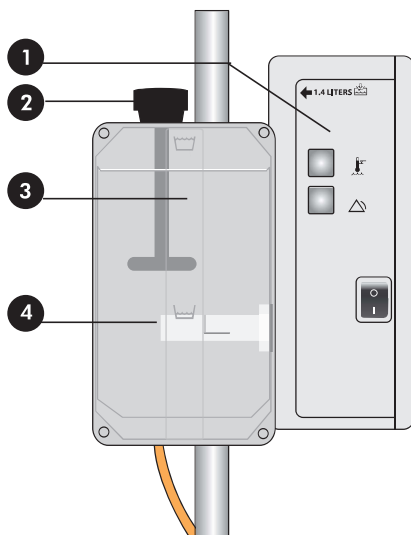**Left Side View**

- 1 Power and Alarm Test Panel
- 2 Fill-port plug
- 3 Reservoir, contains recirculating solution
- 4 Float switch (inside reservoir)

## **HOTLINE® Fluid Warming Set**

HOTLINE® Fluid Warming Sets (L-70, L-70NI, L-80) are individually packed, single-use disposables with a Sterile Fluid Path. The priming volume is 20 ml for the L-70 and L-70NI, and 21 ml for the L-80. The HOTLINE® Fluid Warming Set has a Twin-Tube Connector that plugs into the socket on the right side of the HOTLINE® Warmer. This is the only connection necessary to provide the warming function. The HOTLINE® Fluid Warming Set is easily unplugged from the HOTLINE® Warmer and discarded.

## SECTION 3

# Important Safety Information

This section covers information for prescribers and guidelines for safe use of the HOTLINE® Warmer.

---

## CONTRAINDICATION

Not for use in warming platelets, cryo-precipitates, or granulocyte suspensions.

---

## WARNINGS

*Death or serious injury may occur to the patient or operator if these warnings are not followed.*

- These instructions contain important information for safe use of the product. Read the entire contents of this operator's manual, including Warnings and Cautions, before using this product. Failure to properly follow warnings, cautions, and instructions could result in death or serious injury to the patient.
- The HOTLINE® Fluid Warming Set, L-10, PC-8, and YC-8 are single-use devices and are not intended for re-sterilization.
- Do not use HOTLINE® Fluid Warming Set, L-10, PC-8, and YC-8 if the caps are not securely in place, else the I.V. flow path may not be sterile.
- The HOTLINE® Warmer is for use only with Smiths Medical supplied or approved parts, accessories, and Disposable Sets. The device may not function as intended with the use of unapproved parts, accessories, or Disposable Sets.
- Blood and blood products could contain pathogenic organisms. Failure to follow institutional policy and procedures for biomedical-hazardous materials could lead to exposure to harmful pathogens.
- Set-up, priming, and use require aseptic technique as per applicable institutional policies and procedures.

**WARNINGS** *[continued]*

- Prime the recirculating solution path before connecting to the intravenous extension set. This is to confirm that there is not a breach between the recirculating solution path and intravenous path. If fluid exits the patient end of the HOTLINE® Fluid Warming Set before connecting to the intravenous administration set, remove and replace HOTLINE® Fluid Warming Set.
- Remove all air from the HOTLINE® Fluid Warming Set, L-10, PC-8, and YC-8 before connecting to the patient. Failure to do so may result in introduction of air to the patient.
- To reduce the risk of outgassed microbubbles entering patient vasculature, an L-10 Gas Vent may be used with the HOTLINE® Fluid Warming Set.
- Not for use with pressure devices generating over 300 mmHg. Pressure greater than 300 mmHg may compromise the integrity of the HOTLINE® Fluid Warming Set.
- To prevent a breach between the recirculating solution path and intravenous path, do not use needles greater than 38 mm (1.5") in length when accessing the injection port. If there is a breach between the recirculating solution path and intravenous path, patient illness may occur because of the HOTLINE® Warmer's recirculating solution entering the patient's bloodstream.
- Do not stick the HOTLINE® Fluid Warming Set with needles, as this will breach the I.V. path and compromise the integrity of the patient intravenous line. If a Disposable Set with a breached recirculating solution path/intravenous path is used, then patient illness may occur because of the HOTLINE® Warmer's recirculating solution entering the patient's bloodstream.
- Activation of the Over Temperature warning signal indicates that warming has stopped and immediate operator intervention is required to clear the over temperature condition or to remove the device from service.
- If any visual indicator does not illuminate or the audible signal does not sound, do not use the HOTLINE® Warmer. Remove the device from service immediately.
- Do not operate the HOTLINE® Warmer in the presence of a flammable anesthetic mixture with air, oxygen, or nitrous oxide. The risk of explosion exists if the HOTLINE® Warmer is operated in a potentially explosive environment.

---

**WARNINGS** *[continued]*

- Do not use the HOTLINE® Warmer in high-energy fields such as: MRI, X-RAY, portable and mobile RF communications equipment, and other such devices. The HOTLINE® Warmer may act as a projectile in a strong magnetic field, cause image artifacts, or not function as intended.
- Exposed conductor on MAINS power cord can cause an electrocution hazard. Remove device from service if the MAINS power cord has exposed wires.
- Grounding reliability can only be achieved when the MAINS power cord is connected to a properly grounded receptacle. Risk of electrical shock exists if the equipment is not connected to a properly grounded receptacle.
- Do not mount the HOTLINE® Warmer more than 107 cm (42") above the floor. For convenience, 107 cm (42") is indicated on the HOTLINE® Warmer power cord by a black mark. Mounting the HOTLINE® Warmer above 107 cm (42") may result in instability of the pole and tipping.
- Ensure that the HOTLINE® Warmer clamp is screwed tightly onto the I.V. pole. Failure to securely mount the HOTLINE® Warmer onto the I.V. pole may cause the HOTLINE® Warmer to slide down the I.V. pole.
- Do not use the HOTLINE® Warmer if equipment or Disposable Set malfunction is evident.
- No operator-serviceable parts. All service must be performed by Smiths Medical or competent personnel.
- No modification of this equipment is allowed.
- The HOTLINE® Warmer should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, you should verify normal operation of the HOTLINE® Warmer in the configuration in which it is to be used.
- Common portable and mobile consumer electronic devices may cause interference with the HOTLINE® Warmer. Observe the HOTLINE® Warmer to verify normal operation.
- Facility wiring must comply with all applicable electrical codes. Do not bypass power cord connections. Do not remove a prong from the power cord.

---

**CAUTIONS**

*Malfunction, failure, or damage to the device may occur if these cautions are not followed.*

- **Federal (U.S.A.) law restricts this device to sale by or on the order of a physician.**
  - **Do not autoclave or immerse any part of the HOTLINE® Warmer in liquids, which may cause damage and improper functioning.**
  - **Never use organic solvents (e.g., acetone), strong acids, or bases to clean any portion of the HOTLINE® Warmer.**
  - **Do not place the HOTLINE® Warmer directly under a faucet or use a faucet sprayer to rinse. Never spray cleaning or other fluids into openings on the HOTLINE® Warmer or into the external connectors.**
  - **This device is cooled by convection. Be sure the air vents on the bottom and the back of the device are kept clear.**
  - **Do not fill the HOTLINE® Warmer reservoir with a HOTLINE® Fluid Warming Set in place. Failure to remove the HOTLINE® Fluid Warming Set before the fill procedure may result in an air lock in the HOTLINE® Warmer.**
  - **Medical devices require specific material characteristics to perform as intended. These characteristics have been verified for single use only. Any attempt to re-process the device for subsequent re-use may adversely affect the integrity of the device or lead to deterioration in performance.**
-

---

**Additional WARNINGS and CAUTIONS for Accessories****WARNINGS for the L-10 Gas Vent and L-80 Fluid Warming Set**

- Do not tape over vents, else air will not be vented.
- Not for use with volumetric infusion pumps, hand pumps, or syringes. These may compromise the integrity of the L-10 Gas Vent or HOTLINE® Fluid Warming Set.
- When the L-10 Gas Vent is in use, it should be placed at or below the heart level. Do not raise the gas vent above the patient's heart level. If the gas vent is raised above heart level, air may be entrained into the infusion line, possibly causing air embolism, resulting in serious injury or death.

**CAUTIONS for the L-10 Gas Vent and L-80 Fluid Warming Set**

- This product contains natural rubber latex, which may cause allergic reactions.
-

## SECTION 4

# Assembly Instructions

Read through the instructions completely prior to setting up the HOTLINE® Warmer.

## Step 1 - Unpack the HOTLINE® Warmer

- 1 Open the shipping carton and remove the HOTLINE® Warmer.
- 2 Check the contents of the package to verify the following components are present:
  - HOTLINE® Warmer
  - Operator's Manual
  - HOTLINE® Inspection/Test Form
- 3 Examine the HOTLINE® Warmer for damage. If any components appear damaged, do not use the HOTLINE® Warmer. Contact Smiths Medical for a replacement.

**Note:** After unpacking the HOTLINE® Warmer, recycle packaging material according to hospital policy for recyclable materials.


## Step 2 - Clamp the HOTLINE® Warmer to the I.V. Pole

### WARNINGS


- Ensure that the HOTLINE® Warmer pole clamp is screwed tightly onto the I.V. pole. Failure to securely mount the HOTLINE® Warmer onto the I.V. pole may cause the HOTLINE® Warmer to slide down the pole and may injure the patient or operator.
- Do not mount the HOTLINE® Warmer more than 107 cm (42") above the floor. For convenience, 107 cm (42") is indicated on the HOTLINE® Warmer line cord by a black mark. Mounting the HOTLINE® Warmer above 107 cm (42") may result in instability of the pole and tipping that may injure the patient or operator.

### CAUTION

This device is cooled by convection. Be sure the air vents on the bottom and the back of the device are kept clear.


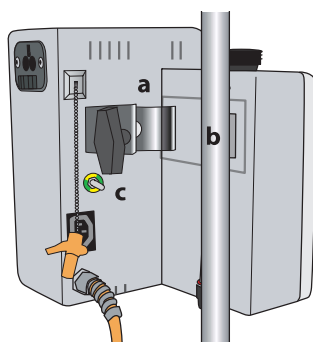


- 1 Slide the clamp **(a)** on the HOTLINE® Warmer over the I.V. pole **(b)** and tighten the clamp screw **(c)** firmly.
- 2 Check the tightness of the HOTLINE® Warmer to ensure it is securely clamped to the pole.

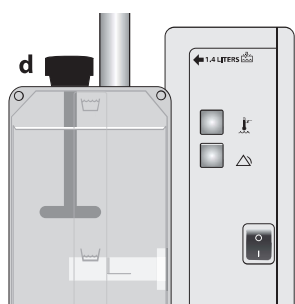

### Step 3 - Disinfect the Reservoir

- 1 Prepare a 0.3% hydrogen peroxide solution by mixing 140 ml of 3% hydrogen peroxide solution and 1,260 ml of distilled water.
- 2 Remove the reflux plug from the socket if required, and then remove the fill-port plug **(d)** and fill the reservoir with 1.4 liters of 0.3% hydrogen peroxide solution.
- 3 Replace the fill-port plug **(d)**.
- 4 Insert a HOTLINE® Fluid Warming Set **(e)** (L-70, L-70 NI, L-80) into the socket.
- 5 Plug the HOTLINE® Warmer into properly grounded power outlet.
- 6 Turn the HOTLINE® Warmer ON and let the solution circulate for a 30-minute disinfection period.
- 7 Turn the HOTLINE® Warmer OFF.

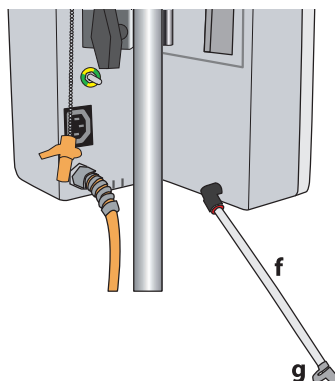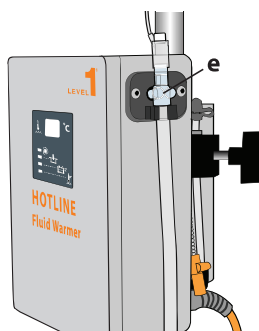

- 8 Invert the drain tube **(f)** and place a container under the end of the tube. Remove the end cap **(g)** and drain the recirculating solution into the container.
- 9 When all the recirculating solution has drained from the reservoir, replace the end cap and insert the drain tube back in the holder.
- 10 Remove the HOTLINE® Fluid Warming Set and discard according to established hospital procedures.

## Step 4 - Fill the Reservoir With Recirculating Solution

### WARNING

Do not fill the HOTLINE® Warmer reservoir with a HOTLINE® Fluid Warming Set in place. Failure to remove the HOTLINE® Fluid Warming Set before the fill procedure may result in an air lock in the HOTLINE® Warmer.

### Recirculating Solution Protocols

Use one of the following solutions for the reservoir.


Recirculating Solution	Preparation	Maintenance
0.3% Hydrogen Peroxide Solution	Mix 140 ml of 3% hydrogen peroxide with 1,260 ml of distilled water.	Replace solution and disinfect reservoir every 12 months.
Distilled Water	Use distilled water.	Replace solution and disinfect reservoir every 30 days.
35% Isopropyl Alcohol Solution	Mix 700 ml of 70% isopropyl alcohol with 700 ml of distilled water.	Replace solution and disinfect reservoir every 30 days.

**Note:** Use distilled water only, not tap water. Failure to do so may cause build-up of mineral deposits in the recirculating solution path, which may impair heater performance.

- 1 Prepare the recirculating solution.
- 2 Remove the fill-port plug (a).
- 3 Fill the reservoir with 1.4 liters of recirculating solution.
- 4 Replace the fill-port plug.

## Step 5 - Perform the Electrical Safety Tests


Perform all applicable electrical safety tests as required per institutional procedure. Refer to Section 9, "Testing", for more information about electrical safety testing.

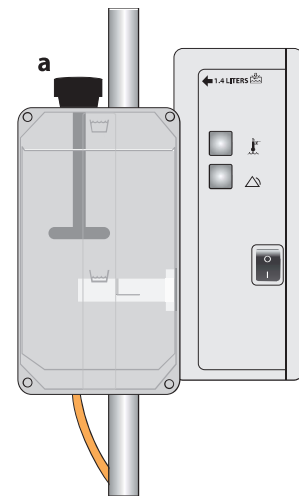

## SECTION 5

# Principle of Operation

HOTLINE® Warmer delivers blood and intravenous fluid at normothermic temperatures under routine, gravity flow rates. Conventional fluid warming systems suffer from cool-down between the warmer and the patient connection. HOTLINE® Warmer overcomes this problem by providing active warming of the patient line all the way to the patient connection.

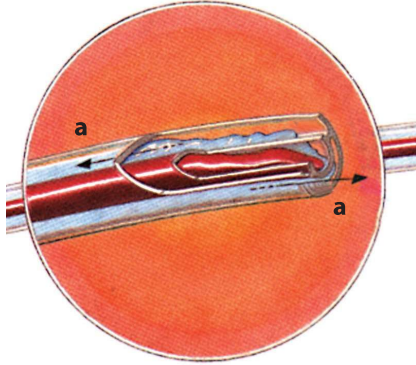


Active warming is achieved by surrounding the sterile intravenous line with a layer of precisely controlled warm recirculating solution (a), thereby protecting the patient line against exposure to cold and eliminating patient line cool-down.

The unique design of the HOTLINE® Fluid Warming Set allows blood and intravenous fluid to be delivered to the patient at normothermic temperature at gravity flow rates to 50-5,000 ml/hr.

## Infusate Delivery Temperatures

The following table shows the typical infusate delivery temperatures at the patient end of an L-70 HOTLINE® Fluid Warming Set.

**Note:** The setpoint temperature of the recirculating solution is 41.9°C.

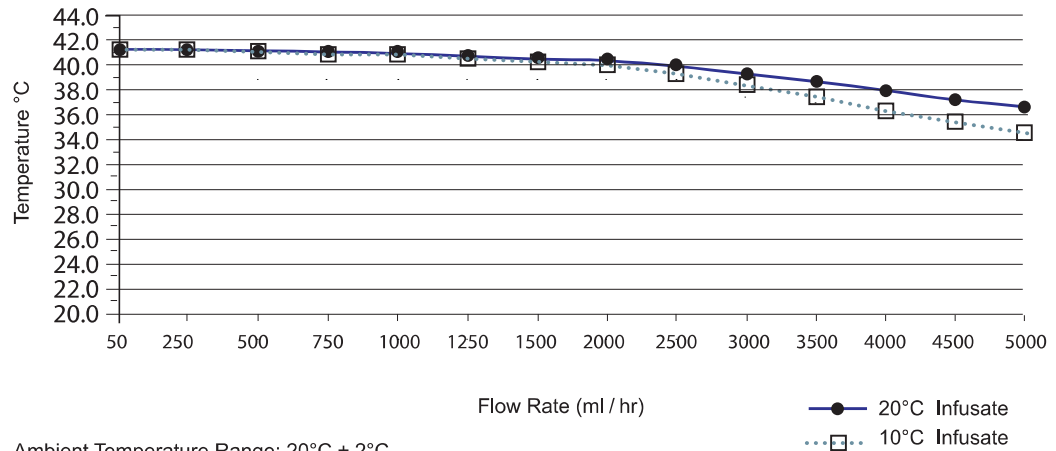

# Operation

This section describes the controls and displays that monitor and control the HOTLINE® Warmer, and the modes of operation.


## Controls and Displays


- Display Panel
- Power and Alarm Test Buttons
- Reservoir Level Display

### Display Panel

The Display Panel is located on the front of the HOTLINE® Warmer and provides continuous information about the operation of the HOTLINE® Warmer. A liquid crystal display (LCD) indicates recirculating solution temperature. Just below the LCD, four light-emitting diodes (LEDs) indicate operation modes for the HOTLINE® Warmer.

- 1 Recirculating Solution Temperature** - The temperature is displayed in degrees Celsius.
- 2 ON/Operation** - The green LED illuminates when the power is turned on and the HOTLINE® Fluid Warming set is properly installed.
- 3 Check Disposables** - The red LED illuminates and an audible attention signal beeps when the HOTLINE® Fluid Warming Set is not properly installed.
- 4 Add Recirculating Solution** - The red LED illuminates and an audible attention signal beeps when the level in the reservoir is low and additional recirculating solution must be added.
- 5 Over Temperature** - The red LED illuminates and an audible warning signal beeps when the recirculating solution is over the acceptable temperature for safe use.

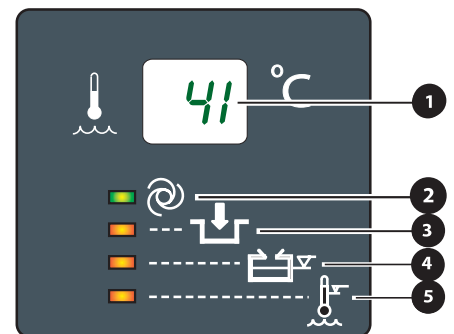


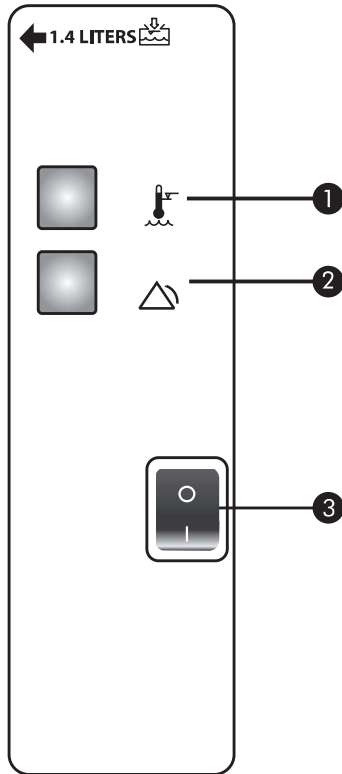

### Power and Alarm Test Panel

The Power and Alarm Test Panel is located on the left side of the HOTLINE® Warmer next to the reservoir. This panel contains two pressure-sensitive buttons that are activated when pressed, and the ON/OFF switch.

- 1 Over Temperature Alarm Test Button** - The Over Temperature Alarm Test is used to confirm the proper operation of the Over Temperature circuitry.
- 2 Alarm Test Button** - The Alarm Signal Test is used to confirm proper operation of the visual and audible alarms.
- 3 Power ON/OFF Switch** - The black switch toggles to turn power ON and OFF.

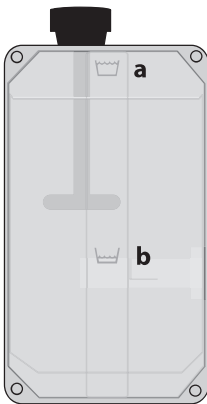

### Reservoir Level Display

The reservoir for the recirculating solution is located on the left side of the HOTLINE® Warmer, next to the Power and Alarm Test Panel. The level of the recirculating solution is visible in the reservoir. Two symbols indicate the maximum (**a**) and minimum (**b**) solution level requirements.

## Modes of Operation


The HOTLINE® Warmer operation is defined in the following modes:

- OFF Mode
- ON/Operating Mode
- Check Disposables Mode
- Add Recirculating Solution Mode
- Over Temperature Alarm Mode

The description of each mode includes a definition of the mode, activation and/or monitoring of the mode, mode characteristics, and method to clear the mode state.


### OFF Mode

The power switch is in the OFF position (**a**) and the HOTLINE® Warmer is turned off.



### ON/Operating Mode

The power switch is in the ON position (**b**) and the HOTLINE® Fluid Warming Set has been properly installed.



#### Mode characteristics

- The green Operating LED (**c**) illuminates.
- The reservoir temperature display will begin to increase.
- The recirculating solution path in the HOTLINE® Fluid Warming Set will automatically prime.



### Check Disposables Mode

The Check Disposables mode indicates a missing or improperly installed HOTLINE® Fluid Warming Set.

#### Mode characteristics


- The green Operating LED on the Display Panel turns off.
- The red Check Disposables LED (**d**) on the Display Panel illuminates.
- The audible alarm sounds (54-59 dB) and repeats approximately every two seconds.
- The recirculating solution stops circulating.



To clear this mode, check that the Twin-Tube Connector on the HOTLINE® Fluid Warming Set is firmly inserted in the socket.

### Add Recirculating Solution Mode

The Add Recirculating Solution mode indicates that the solution level in the reservoir is below its minimum level.



#### Mode characteristics

- The green Operating LED on the Display Panel turns off.
- The red Add Solution LED (**a**) on the Display Panel illuminates.
- The audible alarm sounds (54-59 dB) and repeats approximately every two seconds.
- The recirculating solution stops circulating.

To clear this mode, add recirculating solution to the reservoir.

### Over Temperature Alarm Mode

The Over Temperature Alarm mode indicates that the temperature of the recirculating solution is at or above 43.1°C.



#### Mode characteristics

- The green Operating LED on the Display Panel turns off.
- The red Over Temperature LED (**b**) on the Display Panel illuminates.
- The audible alarm sounds (54-59 dB) and repeats approximately every two seconds.
- The recirculating solution stops circulating.

For instructions to clear this mode, see Section 8, "Troubleshooting".

# Operating Instructions

The Operating Instructions are grouped into five segments. Read through each segment BEFORE performing a procedure.

---

## WARNINGS

- Set-up, priming, and use require aseptic technique as per applicable institutional policies and procedures. Death or serious injury may occur to the patient or operator if this warning is not followed.
- Grounding reliability can only be achieved when MAINS power cords are connected to a properly grounded receptacle. Risk of electrical shock exists if the equipment is not connected to a properly grounded receptacle.
- Do not fill the HOTLINE® reservoir with a HOTLINE® Fluid Warming Set in place. Failure to remove the HOTLINE® Fluid Warming Set before the fill procedure may result in an air lock in the HOTLINE® Warmer.

---

## Step 1 - Set Up the HOTLINE® Warmer

- 1 Check that the level is above the minimum level mark **(a)** on the reservoir. Add recirculating solution to the reservoir through the fill-port if required.
- 2 Check the condition of the HOTLINE® Warmer with a visual inspection before using. Remove from service any HOTLINE® Warmer that shows physical damage.
- 3 Plug the HOTLINE® Warmer into properly grounded power outlet.




## Step 2 - Set Up the HOTLINE® Fluid Warming Set

### WARNINGS

- The HOTLINE® Fluid Warming Set is a single-use device and is not intended for re-sterilization. Death or serious injury may occur to the patient or operator if this warning is not followed.
- Do not use HOTLINE® Fluid Warming Set, L-10, PC-8, and YC-8 if the caps are not securely in place, else flow path may not be sterile and may cause death or serious injury.
- Prime the recirculating solution path before connecting to the intravenous extension set. This is to confirm that there is not a breach between the recirculating solution path and intravenous path. If fluid exits the patient end of the HOTLINE® Fluid Warming Set before connecting to the intravenous extension set, remove and replace HOTLINE® Fluid Warming Set. Death or serious injury may occur to the patient or operator if this warning is not followed.

To set up the HOTLINE® Fluid Warming Set, you will need the following:

- HOTLINE® Warmer
  - Intravenous administration set
  - Intravenous fluid or blood
  - Extension Set, 20 cm (8") or less in length (optional)
- 1 Remove the reflux plug (if present) from the socket on the right side of the HOTLINE® Warmer.
  - 2 Plug the Twin-Tube Connector on the HOTLINE® Fluid Warming Set (**a**) into the socket.
  - 3 Turn ON the power switch.
    - The green Operating LED on the Display Panel illuminates.
    - The recirculating solution temperature display will begin to increase.
    - The recirculating solution path in the HOTLINE® Fluid Warming Set will automatically prime.
  - 4 Remove the end cap and inspect the patient end of the HOTLINE® Fluid Warming Set for leaks to confirm the integrity of the intravenous pathway.

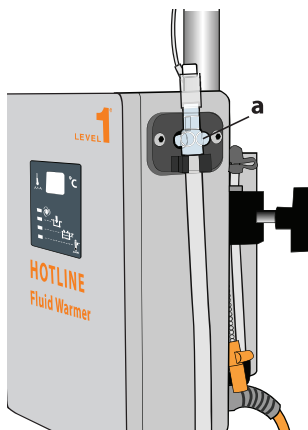

---

## Step 3 - Connect the Intravenous Administration Set

---

### WARNINGS

- Remove all air from the HOTLINE® Fluid Warming Set, L-10, PC-8, and YC-8 before connecting to the patient. Failure to do so may result in introduction of air to the patient, which may contribute to serious patient injury or death.
- To prevent a breach between the recirculating solution path and intravenous path, do not use needles greater than 38 mm (1.5") in length when accessing the injection port. If there is a breach between the recirculating solution path and intravenous path, patient illness may occur because of the HOTLINE® Warmer's recirculating solution entering the patient's bloodstream.
- Do not stick the HOTLINE® Fluid Warming Set with needles, as this will breach the I.V. path and compromise the integrity of the patient intravenous line. If a Disposable Set with a breached recirculating solution path/intravenous path is used, then patient illness may occur because of the HOTLINE® Warmer's recirculating solution entering the patient's blood stream.

- 
- 1 Connect the I.V. fluid and the intravenous administration set to the HOTLINE® Fluid Warming Set.
  - 2 Fully prime the intravenous administration set, the HOTLINE® Fluid Warming Set, and patient extension set (if used).
  - 3 Connect the distal end of the HOTLINE® Fluid Warming Set to the patient's intravenous access site without entrapping air.

## Step 4 - Using the HOTLINE® Warmer

---

### WARNINGS

- Activation of the Over Temperature warning signal indicates that warming has stopped and immediate operator intervention is required to clear the over temperature condition or to remove the device from service. Death or serious injury may occur to the patient or operator if this warning is not followed.
- If any visual indicator does not illuminate or the audible signal does not sound, do not use the HOTLINE® Warmer. Remove the device from service immediately. Death or serious injury may occur to the patient or operator if this warning is not followed.

**WARNINGS** [continued]

- Not for use with pressure devices generating over 300 mmHg. Pressure greater than 300 mmHg may compromise the integrity of the HOTLINE® Fluid Warming Set.


- 1 Wait until the recirculating solution temperature display reaches 41°C, which indicates the HOTLINE® Warmer is ready for use.
- 2 Adjust the rate of I.V. flow using the clamp on the intravenous administration set.

**Note:** Do not kink the Disposable Set. Do not restrict the circulation of the solution through the tubing.

**Step 5 - After Use****WARNING**

Blood and blood products could contain pathogenic organisms. Failure to follow institutional policy and procedures for biomedical-hazardous materials could lead to exposure to harmful pathogens.

- 1 Turn OFF the power switch.
- 2 Remove the HOTLINE® Fluid Warming Set, and insert the reflux plug (a) into the socket.
- 3 After use, handle and dispose of the HOTLINE® Fluid Warming Set in a safe manner according to local guidelines for disposal of contaminated medical waste.
- 4 Wipe down the external surfaces of the HOTLINE® Warmer with mild liquid detergent soap and warm tap water mixture and a soft cloth or sponge. See Section 10, "Maintenance", for more details about cleaning and external disinfection.

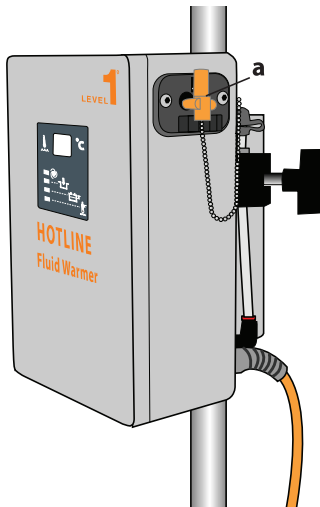**Storage**

Store the HOTLINE® Warmer in a cool, dry place. Do not expose to extreme temperatures. See Section 13, "Specifications and Accessories", for more details.

# Troubleshooting

Only competent personnel should perform any routine maintenance and repairs to the HOTLINE® Warmer.

Problem	Check the following
No power	<ol style="list-style-type: none"> <li>1 Confirm that the HOTLINE® Warmer is plugged in properly.</li> <li>2 Confirm that the power switch is in the ON position. <b>Note:</b> <i>If the HOTLINE® Warmer is plugged in and the power switch is turned ON, the green or red LED will illuminate.</i></li> </ol>
Check Disposables alarm	<p>Confirm that the HOTLINE® Fluid Warming Set is properly installed.</p> <ol style="list-style-type: none"> <li>1 Push the Twin-Tube Connector firmly into the socket on the right side of the HOTLINE® Warmer. <b>Note:</b> <i>Turn OFF the power switch before replacing the HOTLINE® Fluid Warming Set.</i></li> <li>2 If the alarm is not cleared, replace the HOTLINE® Fluid Warming Set. Turn ON the power switch and verify that the alarm has cleared.</li> <li>3 If the alarm is not cleared, remove the HOTLINE® Warmer from service.</li> </ol>
Add Recirculating Solution alarm	<p>Check the level in the reservoir</p> <ul style="list-style-type: none"> <li>• Turn OFF the power switch, remove the HOTLINE® Fluid Warming Set if installed, and add recirculating solution to the maximum level.</li> </ul>
Over Temperature alarm	<ol style="list-style-type: none"> <li>1 Check the HOTLINE® Fluid Warming Set for kinks or other restrictions.</li> <li>2 Check for air lock: <ol style="list-style-type: none"> <li>a Turn the power switch OFF, remove the HOTLINE® Fluid Warming Set, and gently shake HOTLINE® Warmer to dislodge air.</li> <li>b Plug in the HOTLINE® Fluid Warming Set and turn power switch ON.</li> <li>c If the alarm is not cleared, remove the HOTLINE® Warmer from service and return it for repair or replacement.</li> </ol> </li> </ol>
Hot cabinet	<p>Check for blocked air vents on the bottom or the back of the HOTLINE® Warmer. <b>Note:</b> <i>Room temperature above 42°C may cause the HOTLINE® Warmer to shut down and the Over Temperature alarm to activate. In this situation, turn the power switch OFF and allow the HOTLINE® Warmer to cool down before returning it to service.</i></p>

---

<b>Problem</b>	<b>Check the following</b>
Difficult to install the HOTLINE® Fluid Warming Set	Lubricate O-rings in the socket. Refer to Section 10, "Maintenance", for the procedure.
Recirculating solution leaks at the socket where the HOTLINE® Fluid Warming Set plugs into the HOTLINE® Warmer	Replace O-rings. Use the O-ring Replacement Kit: P/N 80-04-001. Refer to Section 10, "Maintenance", for the procedure.
Electrical interference - receiving or transmitting	<ol style="list-style-type: none"><li>1 Move the HOTLINE® Warmer away from the device in question.</li><li>2 Plug the HOTLINE® Warmer into a separate electrical circuit.<ul style="list-style-type: none"><li>• If the problem continues, notify Smiths Medical or your local Smiths Medical distributor.</li></ul></li></ol>

# Testing

The HOTLINE® Warmer should be tested by hospital biomedical personnel prior to placing it in service. All testing and maintenance should be performed by competent personnel. If competent personnel are not available, contact Smiths Medical or your local Smiths Medical distributor.

If the HOTLINE® Warmer and any installed accessories do not pass any of the listed tests, discontinue use of the HOTLINE® Warmer and remove from service. Contact Smiths Medical or your local Smiths Medical distributor.

---

## WARNING

**If any visual indicator does not illuminate or the audible signal does not sound, do not use the Fluid Warmer. Remove the device from service immediately. Death or serious injury may occur to the patient or operator if this warning is not followed.**

---

**Note:** Alarm testing requires a HOTLINE® Fluid Warming Set to be installed and that the HOTLINE® Warmer be turned ON and in the Operating mode.

## Alarm Signal Test


The Alarm Signal Test is used to confirm proper operation of the visual and audible alarm indicators.

- 1 Press and hold the Alarm Test button (a).
- 2 Observe the following:
  - The green Operating LED turns off.
  - Three red LEDs (Check Disposables, Add Solution, and Over Temperature) illuminate.
  - The audible alarm sounds (54-59dB) and repeats approximately every two seconds.



## Over Temperature Alarm Test

The HOTLINE® Warmer should be running at an operating temperature of approximately 41°C to 42°C.



- 1 Press and hold the Over Temperature Alarm Test button **(a)**.
- 2 Observe the following:
  - The recirculating solution Over Temperature Alarm activates at 43°C.
  - The green Operating LED turns off.
  - The red Over Temperature LED **(b)** illuminates.
  - The audible alarm sounds (54-59 dB) and repeats approximately every two seconds.
- 3 Stop pressing the Over Temperature Alarm Test button to stop the test.

## Add Recirculating Solution Test

The HOTLINE® Warmer is equipped with a float switch, which senses the recirculating solution level in the reservoir. When the recirculating solution is too low, the Add Recirculating Solution Alarm will activate.

- 1 Remove the fill-port plug **(c)** on the reservoir.
- 2 Gently depress the float switch **(d)**. (This action will simulate the low solution condition.)

**Note:** Use a non-metal tool to depress the float switch because the float switch contains a magnet.


- 3 Observe the following:
  - The green Operating LED turns off.
  - The red Add Recirculating Solution LED **(e)** illuminates.
  - The audible alarm sounds (54-59 dB) and repeats approximately every two seconds.

## Check Disposables Test

An interlock switch/sensor, located in the socket on the right side of the HOTLINE® Warmer, senses a properly installed HOTLINE® Fluid Warming Set. When the switch does not sense a HOTLINE® Fluid Warming Set, the Check Disposables alarm activates.

- 1 Slowly remove the HOTLINE® Fluid Warming Set (**a**) from the HOTLINE® Warmer socket.
- 2 Observe the following actions:
  - The green Operating LED turns off.
  - The red Check Disposables LED (**b**) illuminates.
  - The audible alarm sounds (54-59dB) and repeats approximately every two seconds.

**Note:** In any alarm condition, the pump should not be running. A small amount of solution dripping from the disconnection is normal and should stop in a few seconds.

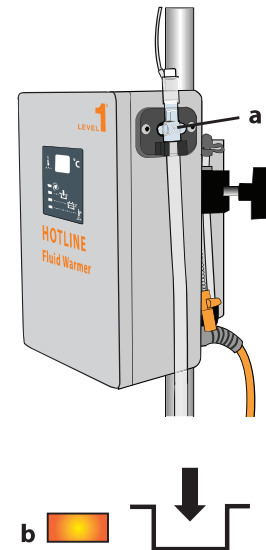

## Temperature Verification of the Recirculating Solution


Use the Level 1® TEMP CHECK Thermometer (HLTA-40) to verify the displayed recirculating solution temperature. Other methods of temperature verification may be inaccurate.

TEMP CHECK provides an accurate reading of the highest temperature of the recirculating solution. Because the temperature of the reservoir is typically 0.5°C to 2.0°C lower than the temperature from the heater, and the temperature of the recirculating solution begins to drop due to the effect of ambient temperature on the HOTLINE® Fluid Warming Set, the highest temperature of the solution is just after it leaves the heater. During the temperature verification test, the TEMP CHECK is positioned on the right side of the HOTLINE® Warmer attached to the socket and senses the solution just after it leaves the heater and before it enters the HOTLINE® Fluid Warming Set.

Refer to the TEMP CHECK HLTA-40 Thermometer Operator's Manual for complete Temperature Verification and Calibration Instructions.

To verify the recirculating solution temperature, you will need the following:

- TEMP CHECK (HLTA-40)
- HOTLINE® Warmer
- HOTLINE® Fluid Warming Set



---

To Verify the Recirculating Solution Temperature:

- 1 Plug the HOTLINE® Warmer into a power outlet.
- 2 Place the TEMP CHECK on the top right corner of the HOTLINE® Warmer and plug it into the socket on the right side of the HOTLINE® Warmer.
- 3 Plug the Twin-Tube Connector on the HOTLINE® Fluid Warming Set into the socket on the right side of the TEMP CHECK.
- 4 Remove the black label from the auxiliary outlet on the back of the HOTLINE® and plug in the TEMP CHECK power cord.

**Note:** *The auxiliary outlet is for use only with Smiths Medical accessories.*

- 5 Turn ON the HOTLINE® Warmer. Allow 15 minutes for the temperature to stabilize.
- 6 If the TEMP CHECK display indicates a temperature between 41°C and 42°C, and the HOTLINE® Warmer display equals the TEMP CHECK display, recirculating solution verification is complete. Refer to the TEMP CHECK Manual for OVERTEMP ALARM verification.
- 7 If the TEMP CHECK display does not indicate a temperature between 41°C and 42°C, refer to the TEMP CHECK Manual for calibration instructions.

---

## Periodic Electrical Testing

Electrical Safety Tests must be performed by competent personnel authorized by the institution to perform such testing. The Safety Tests must be performed and documented at least once per year, or according to institutional policy. These tests include but are not limited to:

- Leakage current
- Ground bond test

**Note:** *All equipment connecting to the device must conform to IEC or ISO standards for requirements for medical electrical systems (e.g., IEC 60601-1 or clause 16 of IEC 60601-1 3Ed.). Any persons connecting additional equipment to the device, is responsible that the device system created as a result complies with the standard requirements for medical electrical systems.*

### Leakage Current

Leakage current must be tested according to methods and pass/fail criteria described in IEC 60601-1. Leakage current must be performed with the heater circuit in the full ON condition. To achieve this condition, perform the test when the reservoir is at room temperature. When the HOTLINE® Warmer is first turned on and the temperature is rapidly rising, but still below 41°C, the heater circuit is in a full ON condition.

**Note:** *The HOTLINE® Warmer is equipped with sensing interlocks. A HOTLINE® Fluid Warming Set is required to correctly operate the HOTLINE® Warmer and perform leakage current testing. Do not defeat the sensing interlocks or try to operate the HOTLINE® without a HOTLINE® Fluid Warming Set in place.*

### Ground Bond Test

Ground bond test must be tested according to methods and pass/fail criteria described in IEC 60601-1.

## SECTION 10

# Maintenance

Only competent personnel should perform any routine maintenance and repairs to the HOTLINE® Warmer. Maintenance is scheduled with each use, every 30 days, and every 12 months. The tasks are described below.

## Maintenance Performed with Every Use

---

### CAUTION

Do not autoclave or immerse any part of the HOTLINE® Warmer in liquids, which may cause damage and improper functioning.

---

Clean and inspect the HOTLINE® Warmer.

### Clean the Exterior

Clean the entire HOTLINE® Warmer after every use.

---

### CAUTIONS

- Never use organic solvents (e.g., acetone), strong acids, or bases to clean any portion of the HOTLINE® Warmer
  - Do not place the HOTLINE® Warmer directly under a faucet or use a faucet sprayer to rinse. Never spray cleaning or other fluids into openings on the HOTLINE® Warmer or into the external connectors.
- 

- 1 To isolate equipment from MAINS, unplug the HOTLINE® Warmer before servicing.
- 2 Visually inspect the HOTLINE® Warmer to ensure there is no visible damage or deterioration of the enclosure such as cracks, or deterioration of the labels and power cord. Do not clean if there is a defect. Contact Smiths Medical or your local Smiths Medical distributor.
- 3 Immerse a soft cloth or sponge as an applicator into the cleaning solution consisting of mild liquid detergent soap and warm tap water mixture. Squeeze out excess solution so that the applicator is not dripping. Wipe or scrub the entire surface of the enclosure and control panels. Use a soft brush to clean the power cord if necessary.

- 4 Rinse a separate soft cloth or sponge in room temperature running potable water. Squeeze out excess water so that the applicator is not dripping. Wipe all of the aforementioned surfaces. Repeat rinsing the cloth or sponge several times with fresh running water during this process to insure all visible residue is removed.
- 5 Dry the item with a hand towel or soft cloth.
- 6 Visually inspect the HOTLINE® Warmer and its components to insure that they have been thoroughly cleaned. Repeat cleaning procedure if necessary.
- 7 After thoroughly cleaning the HOTLINE® Warmer, perform disinfection if required.
- 8 If it is hospital policy to perform disinfection as part of reprocessing, then follow your institution's guidelines for disinfecting of the surfaces of non-critical medical devices. The list below includes low-level disinfectants that are commonly used in the medical community and high-level disinfectants that are claimed by the manufacturer. The effectiveness of these listed disinfectants should be validated using the hospital procedures.

The following disinfectant agents can be used without causing damage to the enclosure:

Low Level Disinfectants:

- fantastik® All Purpose Cleaner

High Level Disinfectants:

- 1.56% Phenol (e.g., Sporicidin®)
  - 3.4% Glutaraldehyde (e.g., CIDEX® Plus)
  - 10% Bleach solution
  - 1% Ammonia solution
  - Surface disinfectants compatible with plastic materials.
- 9 Rinsing of the disinfectant residue should be done using a soft cloth or sponge as the applicator.

### General Inspection


- Check the condition of the HOTLINE® Warmer with a visual inspection before using. Remove from service any HOTLINE® Warmer that shows physical damage.
- If the HOTLINE® Fluid Warming Set does not install easily, lubricate the O-Rings as directed in the following section.

### Disinfect the Reservoir and Change the Recirculating Solution

Disinfect the reservoir and change the recirculating solution every 30 days or every 12 months based on the recirculating solution used for the HOTLINE® Warmer. Refer to the following table for the maintenance schedule.

Recirculating Solution	Preparation	Maintenance
0.3% Hydrogen Peroxide Solution	Mix 140 ml of 3% hydrogen peroxide with 1,260 ml of distilled water.	Replace solution and disinfect reservoir every 12 months.
Distilled Water	Use distilled water.	Replace solution and disinfect reservoir every 30 days.
35% Isopropyl Alcohol Solution	Mix 700 ml of 70% isopropyl alcohol with 700 ml of distilled water.	Replace solution and disinfect reservoir every 30 days.

**Note:** Use distilled water only, not tap water. Failure to do so may cause build-up of mineral deposits in the recirculating solution path, which may impair heater performance.

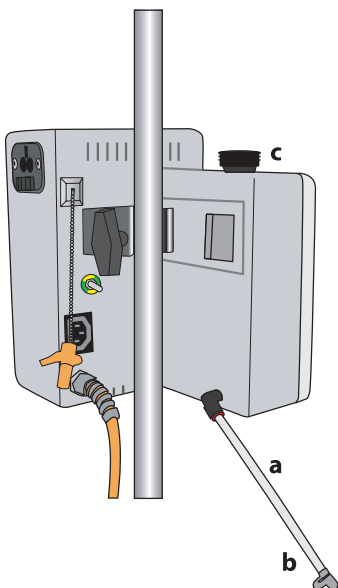


### Disinfect the Reservoir

- 1 To isolate equipment from MAINS, unplug the HOTLINE® Warmer before servicing.
- 2 Remove the drain tube from the holder on the rear of the HOTLINE® Warmer.
- 3 Invert the drain tube (**a**) and place a container under the end of the tube. Remove the end cap (**b**) and drain the recirculating solution into the container.
- 4 When all the recirculating solution has drained from the reservoir, replace the end cap and insert the drain tube back in the holder.
- 5 Prepare a 0.3% hydrogen peroxide solution by mixing 140 ml of

3% hydrogen peroxide solution and 1,260 ml of distilled water.

- 6 Remove the fill-port plug (c), fill the reservoir with the hydrogen peroxide solution, and replace the fill-port plug.
- 7 Remove the reflux plug from the socket if required, and insert a HOTLINE® Fluid Warming Set (d) (L-70, L-70NI, L-80) into the socket.
- 8 Turn the HOTLINE® Warmer ON, and let the recirculating solution circulate for a 30-minute disinfection period.
- 9 Turn the HOTLINE® Warmer OFF and to isolate equipment from MAINS, unplug the power cord.
- 10 Empty the reservoir.
- 11 Remove the HOTLINE® Fluid Warming Set and discard according to established hospital procedures.

These suggested instructions are designed to be used in conjunction with established hospital procedures.

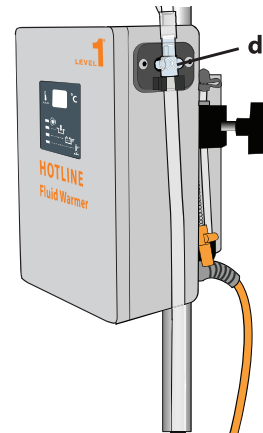

## Add Recirculating Solution

### CAUTION

Do not fill the HOTLINE® Warmer reservoir with a HOTLINE® Fluid Warming Set or a TEMP CHECK in place. Failure to remove the HOTLINE® Fluid Warming Set before the fill procedure may result in an air lock in the HOTLINE® Warmer.

- 1 Prepare the recirculating solution.
- 2 Remove the fill-port plug.
- 3 Fill the reservoir with 1.4 liters of recirculating solution.
- 4 Replace the fill-port plug.


## Maintenance Performed Every 30 Days

### Disinfect the Reservoir and Change Recirculating Solution for Distilled Water and 35% Isopropyl Alcohol Solution

Refer to *Disinfect the Reservoir and Change the Recirculating Solution* procedure in this section.

### Lubricate O-Ring Seals

- 1 Place a small amount of silicone lubricant on a cotton swab.
- 2 Apply silicone lubricant along the O-Rings inside the socket (a) located on the right side of the HOTLINE® Warmer.

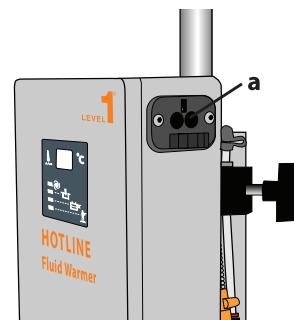


Silicone lubricant is available from Smiths Medical, (Silicone lubricant P/N 80-04-002).

## Maintenance Performed Every 12 Months

### Disinfect the Reservoir and Change Recirculating Solution for 0.3% Hydrogen Peroxide Solution

Refer to *Disinfect the Reservoir and Change the Recirculating Solution* procedure in this section.

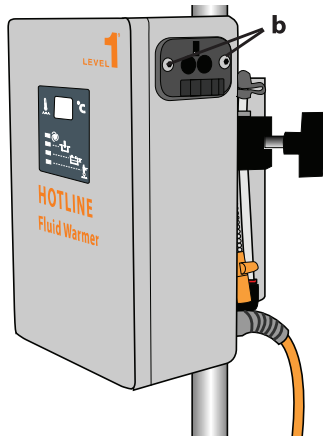

### Replace O-Rings (O-Ring Kit: P/N 80-04-001)

- 1 To isolate equipment from MAINS, unplug the HOTLINE® Warmer before servicing.
- 2 Remove the socket head screws (**b**) with a 0.31 cm (1/8") hex wrench.
- 3 Remove the face plate, being careful not to damage the micro-switch lever.
- 4 Remove the old O-rings and clean the sockets with a cotton swab.
- 5 Apply silicone lubricant to two new O-rings and install into the sockets.
- 6 Reassemble in reverse order, being careful not to damage the micro-switch lever.
- 7 Insert HOTLINE® Fluid Warming Set and power on HOTLINE® Warmer to verify that there are no leaks around the face plate.

### Testing HOTLINE® Warmer Operation

Perform all the tests described in the testing section of this manual. See Section 9, "Testing". The Scheduled Maintenance Checklist below also lists the tests.

## Maintenance Log

All maintenance and testing should be done by competent personnel. Regularly scheduled maintenance ensures proper functioning of the equipment. Refer to the table below for required tasks and frequency of routine maintenance.

### Maintenance Checklist

Task	Every Use	Every 30 Days	Every 12 Months
Clean the Exterior	<input type="checkbox"/>		
General Inspection	<input type="checkbox"/>		
Disinfect the Reservoir and Change Distilled Water or Isopropyl Alcohol solution		<input type="checkbox"/>	
Lubricate the O-Rings		<input type="checkbox"/>	<input type="checkbox"/>
Disinfect the Reservoir and Change the Hydrogen Peroxide Solution			<input type="checkbox"/>
Replace the O-Rings			<input type="checkbox"/>
Alarm Signal Test			<input type="checkbox"/>
Add Recirculating Solution Test			<input type="checkbox"/>
Check Disposables Test			<input type="checkbox"/>
Over Temperature Alarm Test			<input type="checkbox"/>
Verify Temperature Calibration			<input type="checkbox"/>
Electrical Safety Tests			<input type="checkbox"/>

## SECTION 11

# Limited Warranty

Smiths Medical ASD, Inc. (the “Manufacturer”) warrants to the Original Purchaser that the HOTLINE® Blood and Fluid Warmer (the “HOTLINE® Warmer”), not including accessories, shall be free from defects in materials and workmanship under normal use, if used in accordance with this Operator’s Manual, for a period of one year from the actual date of sale to the Original Purchaser. THERE ARE NO OTHER WARRANTIES.

This warranty does not cover normal wear and tear and maintenance items, and excludes any accessory items or equipment used with the HOTLINE® Warmer.

Subject to the conditions of and upon compliance with this Limited Warranty, the Manufacturer will repair or replace at its option without charge (except for a minimal charge for postage and handling) any HOTLINE® Warmer (not including accessories) which is defective if a claim is made during such one-year period.

The following conditions, procedures, and limitations apply to the Manufacturer’s obligation under this warranty:

**A. Parties Covered by this Warranty:** This warranty extends only to the Original Purchaser of the HOTLINE® Warmer. This warranty does not extend to subsequent purchasers. The Original Purchaser may be medical personnel, a hospital, or institution which purchases HOTLINE® Warmers for treatment of patients. The Original Purchaser should retain the invoice or sales receipt as proof as to the actual date of purchase.

**B. Warranty Performance Procedure:** Notice of the claimed defect must be made in writing or by telephone to the Manufacturer as follows: Customer Service Department, Smiths Medical ASD, Inc., 6000 Nathan Lane North, Minneapolis, MN 55442, (800) 258-5361. Notice to the Manufacturer must include date of purchase, model and serial number, and a description of the claimed defect in sufficient detail to allow the Manufacturer to determine and facilitate any repairs which may be necessary. AUTHORIZATION MUST BE OBTAINED PRIOR TO RETURNING THE HOTLINE® WARMER. If authorized, the HOTLINE® Warmer must be properly and carefully packaged and returned to the Manufacturer, postage prepaid. Any loss or damage during shipment is at the risk of the sender.

---

**C. Conditions of Warranty:** The warranty is void if the HOTLINE® Warmer has been 1) repaired by someone other than the Manufacturer or its authorized agent; 2) altered so that its stability or reliability is affected; 3) misused; or 4) damaged by negligence or accident. Misuse includes, but is not limited to, use not in compliance with the Operator's Manual or use with non-approved accessories. Removal or damage to the HOTLINE® Warmer's serial number will invalidate this warranty.

**D. Limitations and Exclusions:** Repair or replacement of the HOTLINE® Warmer or any component part thereof is the EXCLUSIVE remedy offered by the Manufacturer. The following exclusions and limitations shall apply:

1. No agent, representative, or employee of the Manufacturer has authority to bind the Manufacturer to any representation or warranty, expressed or implied.
2. THERE IS NO WARRANTY OF MERCHANTABILITY OR FITNESS OR USE OF THE HOTLINE® WARMER FOR ANY PARTICULAR PURPOSE.
3. The HOTLINE® Warmer can only be used under the supervision of medical personnel whose skill and judgment determine the suitability of the HOTLINE® Warmer for any particular medical treatment.
4. All recommendations, information, and descriptive literature supplied by the Manufacturer or its agents are believed to be accurate and reliable, but do not constitute warranties.

The Manufacturer disclaims responsibility for the suitability of the HOTLINE® Warmer for any particular medical treatment or for any medical complications resulting from the use of the HOTLINE® Warmer. The Manufacturer shall not be responsible for any incidental damages or consequential damages to property, loss of profits, or loss of use caused by any defect or malfunction of the HOTLINE® Warmer.

This warranty gives the Original Purchaser specific legal rights, and the Original Purchaser may have other legal rights which may vary from state to state.

## SECTION 12

# Service

---

**WARNING**

**No operator-serviceable parts. All service must be performed by Smiths Medical or competent personnel. Death or serious injury may occur if this warning is not followed.**

---

All service must be performed by Smiths Medical or competent personnel. Service by any other person or organization voids the warranty and transfers liability for malfunctions of the device to the servicing organization.

## Non-Warranty Work

Devices received that are no longer under warranty can be returned for repair at a cost. The device will be promptly inspected and a verbal estimate of the repair cost will be provided. A purchase order will be required from the original purchaser consistent with the verbal estimate. A written estimate will be provided upon request.

Before returning the HOTLINE® Warmer for service, contact Smiths Medical for Returned Goods Authorization. Be sure that ALL recirculating solution is drained from the device before packing the HOTLINE® Warmer for shipment.

**Note:** *The HOTLINE® Warmer must be cleaned and disinfected for repair shipment or it will be immediately returned as received.*

## Additional Documentation

Upon request Smiths Medical will provide the following documentation:

- Circuit diagrams
- Components parts list(s)
- Description of function
- Service and calibration instructions

## **Disposal Information**

Observe national and local codes or requirements for disposal of contaminated materials and for recycling of solid waste materials that may impact the environment.

## **Service Contacts**

Contact your Smiths Medical Technical Service Department or Smiths Medical distributor at:

### **USA/Canada**

Smiths Medical ASD, Inc.  
6000 Nathan Lane North  
Minneapolis, MN 55442 USA  
Tel: 1 800 258 5361 (US/CA)  
Tel: + 1 614 210 7300

### **European Representative**

Smiths Medical Czech Republic a. s.  
Olomoucká 306, Hranice 1 - Město,  
753 01 Hranice, Czech Republic  
Tel: +44 (0)1233 722100

[www.smiths-medical.com](http://www.smiths-medical.com)

## SECTION 13

# Specifications and Accessories

## System Specifications

<b>Standard Compliance</b>	<b>Guidelines</b>		
Product Safety	IEC 60601-1		
EMC	EN 60601-1-2, FCC 47 CFR Part 15, Class A		
Enclosure Protection	IEC 60529 IP Code: IPX1		
Fluid Warmers	ASTM F2172-02		
<b>Physical</b>	<b>Dimensions</b>		
Height, Overall	24.1 cm	(9.5 inches)	
Width, Overall	21.0 cm	(8.3 inches)	
Depth, Overall	17.8 cm	(7.0 inches)	
Weight, Dry	3.5 Kg	(7.6 lbs)	
Weight, Wet (with recirculating solution)	5.0 Kg	(11.0 lbs)	
Weight, Shipping	3.6 Kg	(7.95 lbs)	
Recirculating Solution Capacity	1.4 L	(0.37 gallons)	
Maximum Height on I.V. Pole	107 cm	(42 inches)	
<b>Environmental</b>	<b>Temperature</b>	<b>Humidity [%]</b>	<b>Atmospheric Pressure</b>
Operation	10°C to 45°C	10 to 95	70kPa to 106kPa
Transportation	-18°C to 60°C	5 to 90	70kPa to 106kPa
Storage	-18°C to 60°C	5 to 90	70kPa to 106kPa
<b>Thermal</b>	<b>Temperature</b>		
Temperature Set Point	41.9°C ± 0.1°C		
Over Temperature Set Point	43.1°C		
<b>Electrical</b>	<b>Type</b>		
MAINS Power Input:			
100V	100VAC, 50/60 Hz, 3.8 Amps		
115V	115VAC, 50/60 Hz, 3.0 Amps		
230V	230VAC, 50/60 Hz, 1.5 Amps		

---

<b>Electrical</b>	<b>Type</b>
MAINS Auxiliary Supply Power Output:	
100V	100VAC, 50/60 Hz, 1.0 Amps
115V	115VAC, 50/60 Hz, 1.0 Amps
230V	230VAC, 50/60 Hz, 0.6 Amps
Protection Against Electrical Shock	Class 1 Equipment, Type BF Applied Part (Disposable set)
Mode of Operation	Continuous
Type of Current	Alternating
Ingress Protection Rating	IPX1
<b>Performance</b>	
Recirculating Solution Temperature	Recirculating solution temperature reaches 37°C from ambient in about 4 minutes
Normothermic Flow Rates	At gravity flow rates to 5,000 ml per hour

---

## Electromagnetic Compliance

HOTLINE® Warmer is certified to be in compliance with the European Communities Council Directive relating to Electromagnetic Compatibility (EMC): (89/336/EEC). Test methods and acceptance criteria as specified in EN 60601-1-2 demonstrate conformance.

<b>Guidance and Manufacturer's Declaration – Electromagnetic Emissions</b>		
Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The HOTLINE® Warmer uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	Note: The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The operator might need to take mitigation measures, such as relocating or re-orienting the equipment.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	
<b>Note:</b> Compliance using 100-240V 50/60Hz with AC power cord of 3.8 m (12.5 ft.).		

### WARNINGS:

- The HOTLINE® Warmer should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, you should verify normal operation of the HOTLINE® Warmer in the configuration in which it is to be used.
- Common portable and mobile consumer electronic devices may cause interference with the HOTLINE® Warmer. Observe the HOTLINE® Warmer to verify normal operation.
- Facility wiring must comply with all applicable electrical codes. Do not bypass power cord connections. Do not remove a prong from the power cord.

<b>Guidance and Manufacturer's Declaration – Electromagnetic Immunity</b>			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 15 kV air	± 8 kV contact ± 15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/output lines	± 2 kV for power supply lines No input/output lines tested	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 0.5 kV, ±1 kV for line to line ± 0.5 kV, ±1 kV, ±2 kV for line to ground	± 1 kV line to line ± 2 kV line to ground	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	100% drop, 0.5 periods, 0°, 45°, 90°, 135°, 180°, 225°, 270°, 315° 100% dip, 250/300 period 30% dip, 25/30 periods	100% drop, 0.5 periods, 0°, 45°, 90°, 135°, 180°, 225°, 270°, 315° 100% dip, 250/300 period 30% dip, 25/30 periods	Mains power quality should be that of a typical commercial or hospital environment. If the operator of the device requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power supply or a battery.
Power frequency (60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

<b>Guidance and Manufacturer's Declaration – Radiofrequency Electromagnetic Immunity</b>			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms 150 kHz to 80 MHz	Portable and mobile RF communications equipment should be used no closer to any part of the system, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. <b>Recommended separation distance:</b> $d = [1.2]\sqrt{P}$
	6 Vrms ISM bands 150 kHz to 80 MHz	6 Vrms 150 kHz to 80 MHz	$d = [0.58]\sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz	10 V/m 80 MHz to 2.7 GHz	$d = [0.35]\sqrt{P}$ 80 MHz to 800 MHz $d = [0.7]\sqrt{P}$ 800 MHz to 2.5 GHz
Radiated RF Proximity Fields	Per 60601-1-2:2014 section 8.10 Table 9.	Per 60601-1- 2:2014 section 8.10 Table 9.	$d = [6/E]\sqrt{P}$ *E is the immunity test level in V/m. Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strength from fixed RF transmitters, as determined by an electromagnetic site survey, <sup>a</sup> should be less than the compliance level in each frequency range. <sup>b</sup> Interference may occur in the vicinity of equipment marked with the following symbol:
<p><b>Note 1:</b> At 80 MHz and 800 MHz, the higher frequency range applies.</p> <p><b>Note 2:</b> These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflected from structures, objects and people.</p>			
<p><sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the system is used exceeds the applicable RF compliance level above, the system should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the system.</p> <p><sup>b</sup> Over the frequency range 150 KHz to 80 MHz, field strengths should be less than 3 V/m.</p>			

## Electromagnetic Environmental Recommendations

Recommended separation distances between portable and mobile RF communications equipment and the HOTLINE® Warmer			
The HOTLINE® Warmer is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the operator of the HOTLINE® Warmer can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the HOTLINE® Warmer as recommended below, according to the maximum output power of the communications equipment.			
Rated Maximum output power or transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d=[3.5/V1]\sqrt{P}$	80 MHz to 800 MHz $d=[3.5/E1]\sqrt{P}$	800 MHz to 2.5 GHz $d=[7/E1]\sqrt{P}$
0.01	0.12	0.12	0.23
0.10	0.37	0.37	0.74
1	1.16	1.16	2.33
10	3.69	3.69	7.38
100	11.66	11.66	23.33

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

**Note 1** At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

**Note 2** The ISM (industrial, scientific, and medical) bands between 150 kHz and 80 MHz are 6.765 MHz to 6.795 MHz; 13.553 MHz to 13.567 MHz; 26.957 MHz to 27.283 MHz; and 40.66 MHz to 40.70 MHz.

**Note 3** An additional factor of 10/3 is used in calculating the recommended separation distance for transmitters in the ISM frequency bands between 150 kHz and 80 MHz and in the frequency range 80 MHz to 2.5 GHz to decrease the likelihood that mobile/portable communications equipment could cause interference if it is inadvertently brought into patient areas.





















**Note 4** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

















## Accessories









REF	Product Description
L-70	HOTLINE® Fluid Warming Set with Injection Port
L-70NI	HOTLINE® Fluid Warming Set without Injection Port
L-80	HOTLINE® Warming Set with L-10 Gas Vent
L-10	Gas Vent
PC-8	T-Connector, 20.3 cm (8") Patient Lead with Injection Port
YC-8	Y-Connector, 20.3 cm (8") Patient Lead with Injection Port

## SECTION 14

# Symbols

Symbol	Meaning
	<b>Caution</b>
	Follow Instructions for Use
	Do not re-use
	Catalog Number
	Serial Number
	Batch Code
	Part Number
	Date of Manufacture
	Use by
	Manufacturer
	Authorized Representative in the European Community
	Contains or Presence of Natural Rubber Latex
	Not made with natural rubber latex
	Contains or Presence of Phthalate: bis(2-ethylhexyl) phthalate (DEHP)
	Sterile Fluid Path, Ethylene oxide gas sterilized
	Type BF Applied Part (Disposable Sets)
	Alternating Current
	Protective earth; protective ground
	Equipotentiality
	Temperature Limitation

Symbol	Meaning
	Humidity Limitation
	Atmospheric pressure limitation
	Quantity
	Do not use if package is damaged
	Keep dry
	Keep away from sunlight
	Collect separately
<b>Rx ONLY</b>	<b>Caution:</b> Federal (U.S.A.) law restricts this device to sale by or on the order of a physician
	Electrical Shock Hazard
<b>IPX1</b>	Protected Against Dripping Water
<b>CLASS 1</b>	Device is a class type 1 equipment
	Protective earth terminal, for maintenance only
	Recyclable Product
	Alarm Test
	Power switch in the ON position
	Power switch in the OFF position.
	Reservoir Temperature Display
	Automatic Operation
	Recirculating Solution Temperature

Symbol	Meaning
	Over Temperature Test (Recirculating Solution Over Temperature)
	Add Recirculating Solution
	Check Disposables, Check Tubing
	Maximum Reservoir Level
	Minimum Reservoir Level
	Device has been tested by TÜV SÜD America, a nationally recognized technical laboratory, to meet all requirements for safety.
	Device has been tested by National Technical Systems, a nationally recognised technical lab, to meet U.S. requirements for safety.
	Warning: Do not stick <b>HOTLINE</b> ® tubing with needles. Patient injury or death result.

# Index

## Numerics

- 0.3% Hydrogen peroxide solution
  - maintenance schedule 30
  - preparation 11, 30
- 35% Isopropyl alcohol solution
  - maintenance schedule 30
  - preparation 11

## A

- Accessories list 40
- Additional documentation 36
- Add Recirculating Solution mode 16
- Add Recirculating Solution test 24
- Add Solution LED 16
- After Use 20
- Alarm signal test 23
- Alarm Test button 14
- Alcohol (isopropyl) solution 11, 30
- Anesthetic use warning 6
- Assembly instructions 9
- Auxiliary electrical outlet 37

## B

- Biohazardous material
  - disposal information 20

## C

- Canada service contact 37
- Cautions 7
  - L-10 Gas Vent 7
- Change the recirculating solution 8
- Check Disposables LED 15
- Check Disposables mode 15
- Check Disposables Test 25
- Clamp for I.V. pole 3
- Clean exterior surfaces 28
- Components 2
  - description 2
- Connect the intravenous administration set 19
- Contents
  - list 9
- Contraindications 5
- Controls 13
- Conventions used in manual 1

## D

- Description
  - components 2
    - HOTLINE Fluid Warming Sets 4
    - HOTLINE Warmer 2
- Disinfect the reservoir 10, 30
- Display Panel 2, 13
  - description 13
- Disposal information 37

- biohazardous materials 20
  - electrical device 37
- Distilled water
  - maintenance schedule 30
- Drain tube 3

## E

- Electrical safety tests 11, 27
- Electrical specifications 38
- Electromagnetic compliance 39
- Electromagnetic environmental recommendations 40
- Environmental specifications 38
- European representative 37

## F

- Fill-port plug 3
- Float switch 3

## G

- Grounding reliability 7, 17
- Guidelines for safe use 5

## H

- HOTLINE Fluid Warming Sets
  - description 4
  - priming volume 4
- Hydrogen peroxide solution
  - preparation 10, 11, 30

## I

- Important safety information 5
- Indications for use 1
- Infusate delivery temperatures 12
- Intravenous administration set
  - connect 19
- Isopropyl alcohol solution 11, 30
- I.V. pole mounting height restrictions 9

## L

- L-10 Gas Vent
  - warnings and cautions 8
- LCD 13
- LEDs 13
- Light-emitting diodes (LEDs) 13
- Liquid crystal display (LCD) 13

## M

- Maintenance 28
  - performed every 12 months 32
  - performed every 30 days 31
  - performed with every use 28
- Maintenance schedule
  - recirculating solution 11, 30
- Modes of operation 15
- Mounting to I.V. pole 9

## N

- Non-Warranty work 36

## O

- OFF mode 15
- ON/Operating mode 15
- Operating LED 15
- Operation modes 13, 15
- O-Rings
  - lubricate seals 31
  - replace 32
- Over Temperature Alarm mode 16
- Over Temperature LED 16
- Over Temperature test 24
- Over Temperature Test button 14

## P

- Performance specifications 39
- Physical specifications 38
- Power and Alarm Test Panel 14
- Power cord 3
- Power ON/OFF switch 14
- priming volume
  - HOTLINE Fluid Warming Sets 4
- Principle of operation 12

## R

- Recirculating solution
  - change 30
  - maintenance schedule 11, 30
  - preparation 11, 30
  - protocols 11
- Reflux plug 3
- Replace
  - O-Rings 32
- Reservoir 3
  - fill with recirculating solution 11
- Reservoir level display 14

**S**

Service 36  
Service contacts 37  
Set Up the HOTLINE Fluid Warming Set 17  
Set Up the HOTLINE Warmer 17  
Socket 2  
Specifications 38  
    electrical 38  
    environmental 38  
    performance 39  
    physical 38  
    thermal 38  
Standard compliance guidelines 38  
Storage 20  
Symbols 41  
System specifications 38

**T**

Temperature  
    display 13  
    Over Temperature Alarm 16  
Temperature verification of the  
    recirculating  
    solution 25  
Testing 23  
Thermal specifications 38  
Troubleshooting 21  
    Add Recirculating Solution alarm 21  
    Check Disposables alarm 21  
    electrical interference 22  
    hot cabinet 22  
    install HOTLINE Fluid Warming Set 22  
    no power 21  
    Over Temperature alarm 21  
    recirculating solution leaks 22


**U**

USA service contact 37  
Using the HOTLINE Warmer 19

**W**

Warnings 5  
    L-10 Gas Vent 8  
Warranty 34

Page intentionally blank

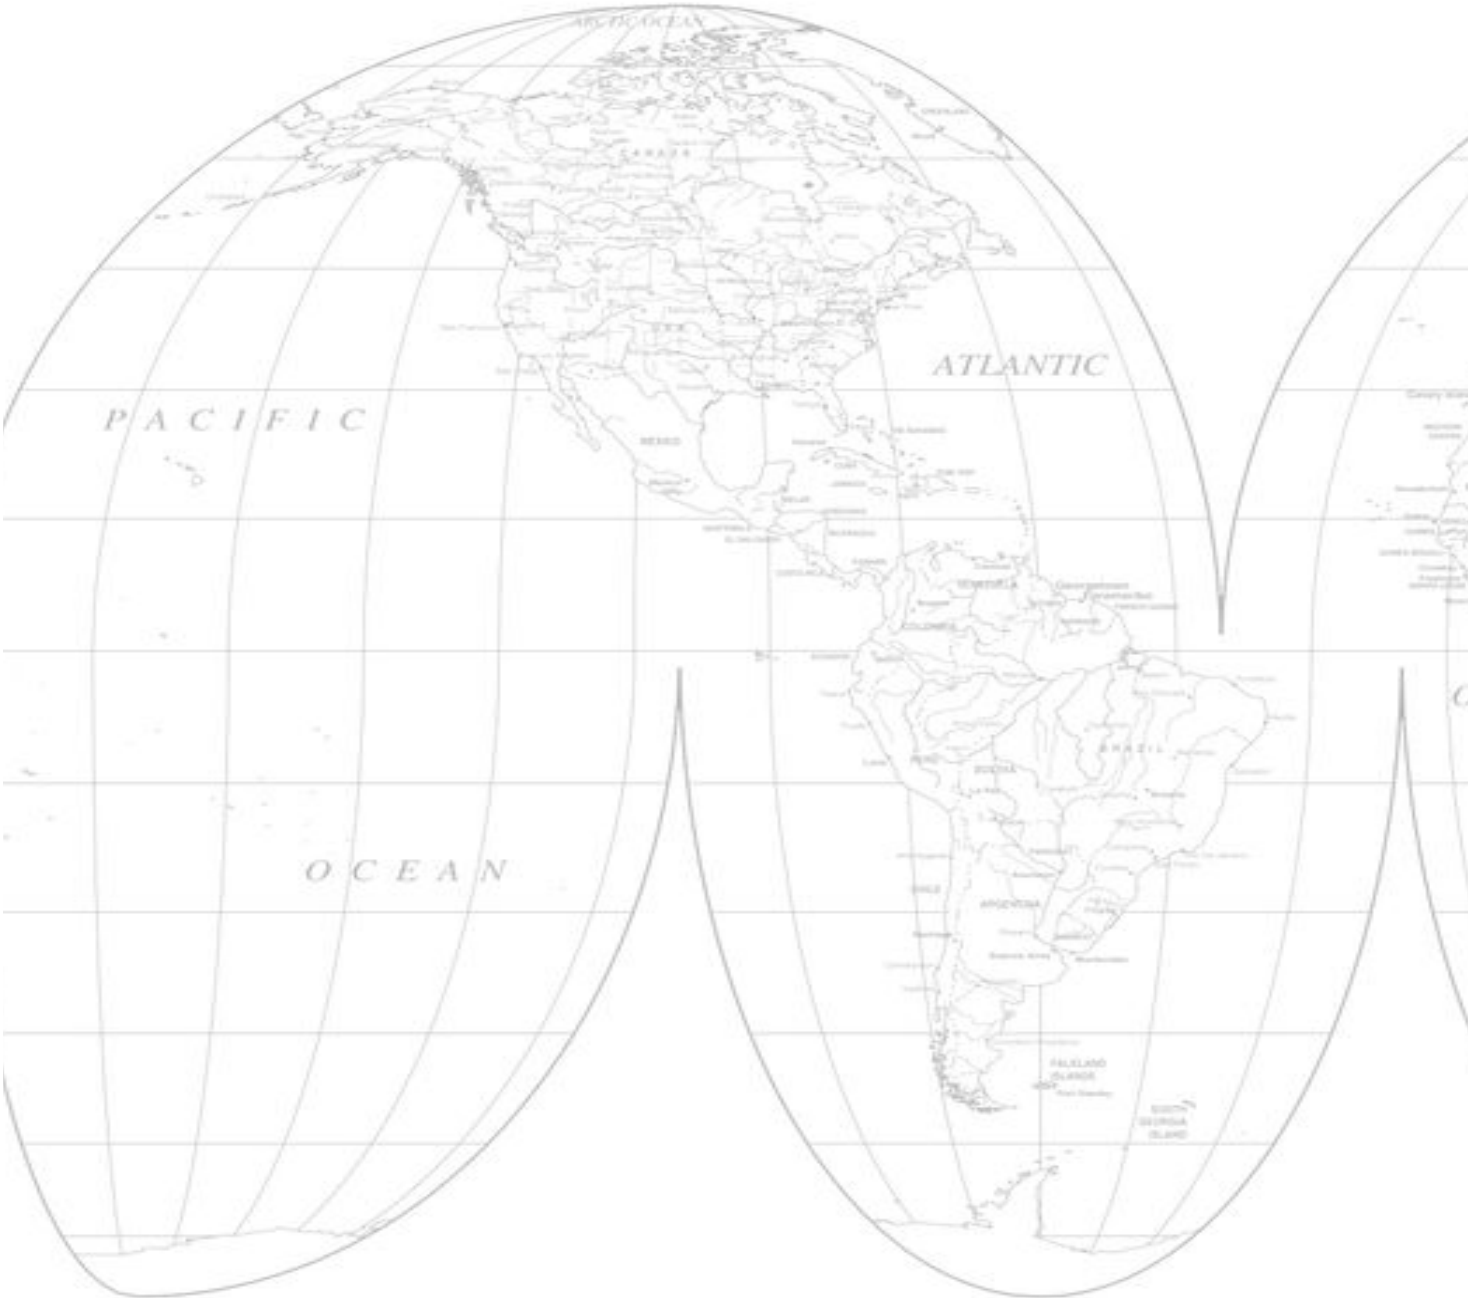

**Manufacturer:**  
**Smiths Medical ASD, Inc.**  
6000 Nathan Lane North  
Minneapolis, MN 55442 USA  
Tel: 1 800 258 5361 (USA/CA)  
Tel: +1 614 210 7300

**EC REP** European Representative:  
**Smiths Medical Czech Republic a. s.**  
Olomoucká 306, Hranice 1 - Město,  
753 01 Hranice, Czech Republic  
Tel: +44 (0)1233 722100

**Rx CE**  
**ONLY 2797**



Origination 12/11/2015  
Last Approved 1/24/2024  
Effective 1/24/2024  
Last Revised 1/24/2024  
Next Review 1/23/2026

Owner Danielle Graber:  
Mgr Laboratory Services -  
Phlebotomy  
Area/Department Laboratory  
Applicability Munson  
Healthcare Systemwide  
Tags Policy

# LAB GEN: Patient Identification for Laboratory Specimen Collection

## Purpose

To provide accurate identification of patients, eliminating related medical errors and patient harm. Identification (ID) of the patient is an on-going process that begins when the patient enters the hospital and continues throughout the patient's stay. To maintain and facilitate patient care and safety and to ensure accurate and reproducible laboratory results, the labeling of laboratory samples will be consistently completed at the point of care.

## Definition

1. **Point of Care:** within close proximity of the draw site; meaning at the patient's bedside or similar area (i.e. next to the drawing chair).

## Policy

- A. Patients are identified by two (2) identifiers at the point of care. All samples are adequately and permanently labeled immediately upon collection at the point of care.

## Identification Guidelines

- A. Two aspects of patient ID must be verified prior to specimen collection:
  1. **Inpatients (includes Emergency Room (ER) patients)**

- a. Scan the patient's ID band located on the patients' wrist or ankle with the PDA system. Ask the patient to state their legal name (First & Last) and date of birth (DOB). Compare their response to the information on the PDA system & patient ID band.
- b. If the PDA system is unavailable compare Sunquest label or chart sticker to the patient ID band located on the patients' wrist or ankle. Ask the patient to state their legal name (First & Last) and DOB. Compare their response to the information on the Sunquest label or chart sticker & patient ID band.
- c. Note: For patients who are unable to verbalize two aspects of ID, verify ID with a caregiver or family member whenever practical.

## 2. Outpatients

- a. Ask patient to state the following information:
  - i. Name: (First and Last legal )??
  - ii. DOB
- b. Verify this information with that on all paperwork provided including the lab requisition(s).

## Labeling Guidelines

- A. Immediately upon collection all samples must be permanently labeled with two patient-specific identifiers:
  1. Affix a sunquest label, chart sticker, or hand write full legal name and second unique ID number (medical record #). If the medical record # is unknown or is not available, acceptable 2nd identifiers are the patient's DOB, account number, office chart number, social security number.
  2. Affix labels vertically down blood tubes and horizontally across other collection containers.
- B. If second label is required, the first permanent label may be covered but not removed. Double check full name and date of birth when applying second label.
- C. Samples must be labeled in the patient's presence. Do not move samples or allow patient to leave the area before labeling the samples.

## Pretransfusion Specimen Labeling Guidelines

- A. Immediately upon collection pretransfusion blood specimens are labeled at the time of specimen collection in the presence of the patient with:
  1. Patient's first and last name
  2. Unique identification number (medical record #)
  3. Date and time of collection
  4. Initials of individual collecting the specimen if not Sunquest label

- B. Sunquest Label, Chart Label, or hand labeled with black or blue ink is acceptable for labeling pretransfusion specimens.
- C. Pretransfusion blood specimen collectors are recorded in the laboratory information system. All phlebotomists have a Tech ID code unique to employee. For non-laboratory staff collections, initials of collector are recorded in the laboratory information system as a comment.

## Additional Information on Specimen Container(s) when Applicable

- A. Specimen Source (such as cultures)
- B. Collection Duration (12 or 24 hours for timed urine specimens)
- C. Collection Time for Serial Draws (30 minutes, 1 hour, 2 hours, 3 hour)
- D. Tube Number in Order of Draw (#1, #2, #3 for spinal fluid tubes)
- E. Preservative Added (acetic acid preservative added to a 24-hour urine container)

## Glass Slides

- A. Glass slides must be labeled with the patient name. A second identifier is preferred, but the name only is acceptable.

## Approval Signatures

Step Description	Approver	Date
System Policy Oversight Committee	Terri Fries: Document Mgmt Spec	1/24/2024
Lab Medical Director	William Kanner	1/24/2024
Document Owner	Danielle Graber: Mgr Laboratory Services	10/20/2023

## Applicability

Cadillac Hospital, Charlevoix Hospital, Grayling Hospital, Kalkaska Memorial Health Center, MHC Corporate (Home Health, Dialysis, NMSA, etc.), Manistee Hospital, Munson Medical Center, Otsego Memorial Hospital, Paul Oliver Memorial Hospital

## Standards

No standards are associated with this document

COPY



**Procedure:** Lumbar and ventricular drain - LimiTorr Drainage System (MUNSON)  
**Checklist:** Lumbar and ventricular drain - LimiTorr Drainage System (MUNSON)  
**Evaluator's Name:** \_\_\_\_\_ **Examinee's Name:** \_\_\_\_\_  
**Evaluator's ID:** \_\_\_\_\_ **Examinee's ID:** \_\_\_\_\_  
**Evaluator's Dept:** \_\_\_\_\_ **Examinee's Dept:** \_\_\_\_\_  
**Date:** \_\_\_\_\_ **Meets criteria/Does not meet criteria:** \_\_\_\_\_

**Select Evaluation Method:**

- Clinical Observation  Documentation Review
- Demonstration  Verbalization

**Lumbar and ventricular drain - LimiTorr Drainage System (MUNSON)**

<b>ATTACH TO POLE</b>
<input type="checkbox"/> Bring IV pole, with the LimiTorr pole mount assembly from equipment storage room (neuro cart), to patient's bedside to attach drainage bag system.
<input type="checkbox"/> Remove sliding bracket from bag.
<input type="checkbox"/> Attach sliding bracket to system by inserting the sliding bracket into the hole behind burette top cap.
<input type="checkbox"/> Place the LimiTorr system on the pole mount assembly. insert manifold into slot on pole mount. When properly connected, the yellow indicator on pole mount will align with the drip level.
<b>PRIME THE SYSTEM</b>
<input type="checkbox"/> Check that all fittings are tightened. Turn the pressure transducer stopcock to "open" to the patient line.
<input type="checkbox"/> Attach 10ml syringe with preservative-free normal saline to transducer stopcock port and prime tubing of patient line to catheter connection.
<input type="checkbox"/> Once the line is primed, replace sterile end cap.
<input type="checkbox"/> Turn stopcock to "off" to patient line.
<input type="checkbox"/> Keeping the 10ml syringe attached, turn transducer stopcock to "open" to burette and "closed" to the patient. Prime tubing, allowing 2-3ml to collect in burette.
<input type="checkbox"/> Drain 2-3ml into drainage bag. Do not fully drain out tube between burette and bag after priming.
<input type="checkbox"/> Remove 10ml syringe and replace with sterile end cap.
<b>SET PRESSURE LEVEL</b>

**Caution: The height of the drainage system, relative to the patient, controls the drainage rate.**

Use laser level or string line level to align the zero reference on the pole mount with the patient landmark ordered by physician (i.e. Tragus, insertion site, etc...)

Set pressure height by aligning the yellow indicator with the drainage level prescribed (cm H<sub>2</sub>O or mm Hg) by moving the sliding bracket. Secure bracket with thumb screw.

Turn stopcock to "open" to drain.

### **LASER LEVEL INS400L INSTRUCTIONS**

**Caution: Do not stare in laser light beam. Do not point at reflective objects.**




Point arrow on level towards the patient.

Ensure laser is level with the pole by adjusting the level so the bubble is centered in-between the two lines on the top of the level.

Press the power switch on.

Adjust height of pole mount so that the light beam is aligned with the patient's anatomical reference point ordered by physician.

Light beam automatically turns off in 30 seconds.



# Malignant Hyperthermia

Bradley Beaman, PharmD, BCPS  
Megan Greenway, MSN, RN, CNOR  
Aaron Kurjan, DO, Medical Director MMG Anesthesia  
Jeannette Reynolds, MSN, RN, CPAN  
Pat Wyers, BSN, RN, CNOR

April 2025



## Goals and Objectives

### Goals

To assist staff in recognizing signs and symptoms of malignant hyperthermia (MH) to be able to implement treatment options.

To increase awareness of the Malignant Hyperthermia Association of United States (MHAUS).

### Objectives

1. List the signs of malignant hyperthermia (MH).
2. State which patients are more conducive to the development of this crisis.
3. Demonstrate knowledge and understanding of administering dantrolene sodium (Ryanodex).
4. Describe management of an MH crisis to include cooling measures, electrolyte imbalances, and dysrhythmias.

Course contains videos - use



or



Page n of nn



## What is Malignant Hyperthermia?

MH is a genetically inherited disorder of skeletal muscle that predisposes susceptible individuals to a life-threatening adverse reaction upon exposure to some anesthetic agents.

It leads to a hypermetabolic crisis manifesting as metabolic and respiratory acidosis, tachycardia, cardiac arrhythmias, skeletal muscle rigidity, and heat production.

Although the occurrence of an MH crisis is rare, incidence varies per geographic location which includes Michigan.



## Malignant Hyperthermia

While most cases of MH occur during general anesthesia, the one-hour period immediately following surgery (including the recovery room) is also a critical time.

In addition, MH can occur if trigger anesthetics and/or succinylcholine are used in any location, such as EDs, dental surgeries, surgeon's offices, or ICUs.



## Malignant Hyperthermia *(cont.)*

Triggers for MH include:

- Inhaled general anesthetics (e.g. desflurane, enflurane, halothane, isoflurane, sevoflurane)
- Succinylcholine
- Exertional heat or exercise (rare)



## MH Susceptible Patients

Currently, no simple diagnostic test is available for screening the general public.

Patients with a history of MH, family history, or even possible history are treated as though they are MH susceptible.

### Screening:

- Scheduled cases will be screened prior to surgery.
- Emergent cases will be screened prior to induction when patient condition or family presence allows.
- Screening should include family or personal history of MH and/or complications from anesthesia.



## Pre-Procedure Prep

During the preprocedural screening, if a patient has been identified as MH susceptible, the following preparation is needed:

- Anesthesia/providers create a detailed plan considering alternative anesthetic agents.
- When possible, schedule the patient as a first case.
- Notify all post-procedure destinations.
- Place the MH cart outside of the procedure room.



## Clinical Features

The sequence and timing of clinical manifestations may vary from patient to patient.

- Unexplained tachycardia or arrhythmias (usually ventricular tachycardia and premature ventricular contractions) - **Early Sign**
- Unexplained increase in end-tidal carbon dioxide (EtCO<sub>2</sub>) - **Early Sign**
- Tachypnea or breathing over the ventilator - **Early Sign**
- Sinus tachycardia - **Early Sign**
- Masseter muscle or generalized muscle rigidity - **Early Sign**
- Hyperkalemia - mixed metabolic/respiratory acidosis - **Early Sign**
- Rapidly rising body temperature (hyperthermia) - **Late Sign**
- Myoglobinuria - **Late Sign**
- Rhabdomyolysis - **Late Sign**
- Disseminated intravascular coagulation (DIC) - **Late Sign**

### Pediatric patients







- Sinus tachycardia, hypercarbia, rapid temperature increase, and skin mottling; may not see muscle rigidity in pediatrics



Please complete the activity before moving on.

## Response to an MH Crisis

If a MH crisis is suspected, immediately take the following steps:  
(Click each arrow to view the information.)

-  Call/page anesthesia provider STAT if not present.
-  Discontinue volatile agents (inhaled general anesthetics and/or Succinylcholine).
-  Obtain the MH Cart/Bag and dantrolene (Ryanodex or Dantrium).
-  Obtain MH Crisis Checklist from MH Cart/Bag and follow the guidelines on the checklist.
  1. Master copies of hospital specific MH crisis checklists are attached to the MHC PolicyStat - Malignant Hyperthermia Guidelines.
-  Contact the Malignant Hyperthermia Association of the United States (MHAUS) for additional support.
-  Contact Pharmacy & Phlebotomy to assist, as needed.

Page n of nn



## MH Initial Treatment

- Hyperventilate with 100% oxygen at flows of 10ml/min.
  - If available, insert activated charcoal filters into the anesthesia breathing circuit.
- Administer initial dose of dantrolene (Ryanodex or Dantrium) 2.5 mg/kg IVP
- Establish large bore IV access (avoid hands), infuse Dextrose 5% (D5W) or 0.9% sodium chloride.
  - Avoid Lactated Ringer's and Normasol, which contain calcium.
- Continue patient monitoring of ECG, pulse oximetry, capnometry, and core body temperature.



## MH Crisis Medications

- Dantrolene sodium IV (Ryanodex, Dantrium)
- Preservative-free sterile water for injection (in vials)
- 8.4% sodium bicarbonate
- 10% calcium chloride
- 50% dextrose
- 2% lidocaine (amiodarone is also acceptable)
- Regular insulin, 100 unit/mL (refrigerated)
- Normal saline solution (at least 3,000 mL, refrigerated)
- D5W



## Dantrolene Sodium

Dantrolene sodium is available as a solution (Dantrium), or as a suspension (Ryanodex) once reconstituted, for treatment of MH.

### Product Comparison

	Dantrium	Ryanodex
Vial strength	Each vial 20 mg	Each vial 250 mg
Reconstitution per vial	60 ml of sterile water preservative free yields 0.33 mg/ml	5 ml of sterile water preservative free yields 50 mg/ml
Time to reconstitute	15-20 minutes for 13 vials	<1 minute for 1 vial
# Vials/per dose	13-18 vials	1-2 vials
Color	<b>Shaken until solution is clear</b>	<b>Uniform orange color</b>
Dose	2.5 mg/kg	2.5 mg/kg

You must watch the video to advance.



## Dantrolene Sodium (Ryanodex)

### Mixing and Administration Instructions:

- Each vial is to be reconstituted with 5 mL of sterile water (NO preservative/NO bacteriostatic agent).
- Mix thoroughly.
- Draw up patient-specific, weight-based dose (2.5 mg/kg).
- Administer IVP into a large bore IV (avoid hand) of 0.9% normal saline or D5W solution; flush line after dose is given.
- Has potential for tissue necrosis with extravasation.

### Ryanodex Video

Click [here](#) to watch a 4½ minute video on how to mix and administer Ryanodex.

## Dantrolene Sodium (Ryanodex) *(cont.)*

Dosing chart is on the MH cart, and also comes with the vial of Ryanodex.

Maximum cumulative dose is 10 mg/kg

### DOSAGE SCHEDULE TO TREAT MH

- Based on recommended loading dose of 2.5 mg per kg<sup>1</sup>
- Chart calculated using 250 mg vials of RYANODEX® (dantrolene sodium) for injectable suspension reconstituted with 5 mL of sterile water for injection USP (without a bacteriostatic agent)<sup>2</sup>
- In case of emergency, contact the 24-hour MHAUS Hotline at 800.644.9737

#### RYANODEX® DOSAGE CHART<sup>3</sup>

Patient's weight in kg	Patient's weight in pounds	Number of 250 mg vials to open	mg dosage needed	mL of reconstituted RYANODEX® to administer
5	11	1	12.5 mg	0.25 mL
10	22	1	25.0 mg	0.50 mL
15	33	1	37.5 mg	0.75 mL
20	44	1	50.0 mg	1.00 mL
25	55	1	62.5 mg	1.25 mL
30	66	1	75.0 mg	1.50 mL
35	77	1	87.5 mg	1.75 mL
40	88	1	100.0 mg	2.00 mL
45	99	1	112.5 mg	2.25 mL
50	110	1	125.0 mg	2.50 mL
55	121	1	137.5 mg	2.75 mL
60	132	1	150.0 mg	3.00 mL
65	143	1	162.5 mg	3.25 mL
70	154	1	175.0 mg	3.50 mL
75	165	1	187.5 mg	3.75 mL
80	176	1	200.0 mg	4.00 mL
85	187	1	212.5 mg	4.25 mL
90	198	1	225.0 mg	4.50 mL
95	209	1	237.5 mg	4.75 mL
100	220	1	250.0 mg	5.00 mL
105	231	2	262.5 mg	5.25 mL
110	242	2	275.0 mg	5.50 mL
115	253	2	287.5 mg	5.75 mL
120	264	2	300.0 mg	6.00 mL
125	275	2	312.5 mg	6.25 mL
130	286	2	325.0 mg	6.50 mL
135	297	2	337.5 mg	6.75 mL
140	308	2	350.0 mg	7.00 mL
145	319	2	362.5 mg	7.25 mL
150	330	2	375.0 mg	7.50 mL

<sup>3</sup> Labeled dose range of 1 to 10 mg/kg with a maximum cumulative dose of 10 mg/kg. If the physiologic and metabolic abnormalities of MH continue, administer additional doses.<sup>1</sup>



# Dantrolene Sodium (Ryanodex) Locations

## Cadillac

MH Cart

## Charlevoix

- MH Cart
- Pharmacy

## Grayling

MH Cart

## Manistee

MH Cart

## Otsego Memorial Hospital


- Anesthesia Pyxis
- ICU Pyxis

## Paul Oliver Memorial Hospital

MH Cart

## MMC

- 2 vials: OR 2<sup>nd</sup> floor in the MH Cart
- 2 vials: OB (Recovery Room) Pyxis
- 2 vials: Basement Pharmacy

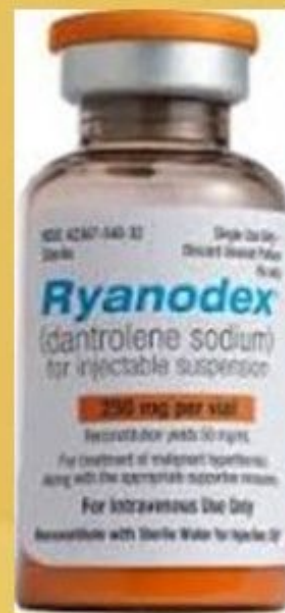



# MH Crisis Checklist

Please refer to your facility-specific MH Crisis Checklist and policy for Malignant Hyperthermia treatment and management.



**Web Window**

[https://mobile.mhc.net/Malignant Hyperthermia Crisis Checklist 2022.pdf](https://mobile.mhc.net/Malignant%20Hyperthermia%20Crisis%20Checklist%202022.pdf)



## Recommended MH Supplies

### **Important - Know the location of your hospital's MH supplies.**

- Charcoal filters
- Variety of syringes, including (3) 5mL syringes and (3) 60 mL syringes
- IV catheter supplies (large bore)
- Central venous access catheter kits (appropriate sizes for patient population)
- Transducer kits for arterial and central venous catheters
- Arterial blood gas (ABG) kits and syringes (3 mL) for blood gas analysis or point of care monitors
- Pressure bag
- Core temperature probes
- Bucket for ice and cold packs
- Large Steri-Drape™ to cover surgical wound
- Urinary catheter kit
- Urine collection container for myoglobin level
- Small and large plastic bags
- Test strips for urine hemoglobin
- Variety of blood collection tubes




## Additional Equipment

- Capnography
- Cooling blanket
- Emergency equipment:
  - Crash cart
  - Defibrillator
  - Intubation supplies
  - Mechanical ventilator
  - Handheld resuscitation bag with mask



## MH Supportive Therapy

- Cool patient, as needed, based on body temperature using ice packs to neck, axilla or groin, cooling blankets, chilled intravenous solution, or lavage.
- Obtain lab work, including blood gas.
- Re-dose dantrolene based on patient response.
- Treat respiratory and metabolic acidosis, hyperkalemia, and dysrhythmias, as needed (avoid calcium channel blockers).
- Monitor renal function and treat myoglobinuria, if needed.
- Provider should consider insertion of an arterial line, central venous catheter, and/or a pulmonary artery catheter.




## Transferring a MH Suspected or Confirmed Patient

- The anesthesia provider will determine the location to best manage patient care during the acute phase (e.g., inpatient facility Post Anesthesia Care Unit (PACU) or critical care unit).
- Notify house supervisor/admitting for bed placement needs, as applicable.
- The anesthesia provider will arrange the transfer and accompany the patient, as needed.



## Post-MH Crisis

- Observe the patient for at least 24 hours on a critical care unit.
- Monitor ABGs, electrolytes, calcium, clotting studies, myoglobin, urine output and color, and other studies as ordered.
- Key indicators of stability include:
  - EtCO<sub>2</sub> is declining or normal
  - Heart rate is stable
  - Hyperthermia is resolving
  - Generalized muscle rigidity has resolved
  - Restock MH cart or bag
- Ensure additional vials of dantrolene (Ryanodex or Dantrium) are readily available.



## Post-MH Crisis Complications

- Dantrolene sodium (Ryanodex) is associated with flushing, drowsiness, voice disorders, dysphagia, and nausea.
  - Symptoms may persist up to 48 hours post-dose.
- Rhabdomyolysis
  - Urine becomes cola-colored (dark red or brown).
  - Patient may c/o muscle pain.
  - **Immediately** notify attending provider and anesthesia provider.
- Paralysis, blindness, renal failure, reoccurrence of syndrome, muscle weakness, multi-organ failure, and/or death
  - Patients should not ambulate without assistance until normal strength and balance has returned.
- Obstetrical cases
  - Dantrolene sodium (Ryanodex) readily crosses placenta - may lead to side effects in unborn child.
  - Notify the obstetrician and pediatrician of dantrolene sodium (Ryanodex) administration.



## Documentation and Reporting

- A. Notify the unit manager and director of the event.
- B. Document event on unit-based patient care records (EMR).
- C. Complete a facility occurrence report (e.g., VOICE) under "adverse medication event".
- D. Anesthesia Services should review each case and consider contributing information to the MHAUS.





# MH Guidelines



**Web Window**

<https://munsonhealthcare-all.policystat.com/policy/14063752/latest>



## Malignant Hyperthermia Association of the United States (MHAUS)


Mission: To promote optimum care and scientific understanding of MH and related disorders.

The MHAUS Association provides:

- Resources for healthcare professionals
  - Education and research
- Patient/family teaching re: MH precautions, susceptibility, and testing centers

Visit <http://www.mhaus.org> for healthcare provider and public education materials.

For support during an MH crisis,  
call the 24-hour **MH Hotline**  
1-800-644-9737





## References

Association for PeriOperative Registered Nurses (AORN). (2025). Malignant Hyperthermia. AORN eGuidelines+.

<https://www.aornguidelines.org/guidelines?bookid=2260>

Malignant Hyperthermia Association of the United States (MHAUS). (2025). Healthcare Professionals. Malignant Hyperthermia Association of the United States.

<https://www.mhaus.org/healthcare-professionals/>

Lippincott Solutions. (2024, May 20). Malignant hyperthermia patient care, OR. Lippincott Procedures. <https://procedures.lww.com/lnp/view.do?pld=723770&hits=malignant,hyperthermia&a=false&ad=false&q=malignant%20hyperthermia>



Origination 1/18/2011  
Last 5/15/2023  
Approved  
Effective 5/15/2023  
Last Revised 5/15/2023  
Next Review 5/14/2026

Owner Kerry Kole:  
Medical Director  
Area/  
Department Trauma Services  
Applicability MMC  
Tags Procedure

## Massive Transfusion Protocol

### Purpose

To provide a process in the case of a massive transfusion.

### Policy

### Indications

- A. Massive blood loss and profound hemorrhagic/hypovolemic shock.
- B. Triggers:
  - 1. Greater than 6 units packed red blood cells (PRBC) transfused within 2 hours.
  - 2. Hemodynamically unstable patient with identified or suspected coagulopathy of trauma or disseminated intravascular coagulopathy (DIC)
  - 3. Any time at the discretion of the trauma surgeon / intensivist.
  - 4. Assessment of blood consumption (ABC) score of greater than or equal to 3 (total possible score 4)
    - a. Penetrating mechanism (no= 0; yes= 1)
    - b. Emergency department (ED) systolic blood pressure less than 90 mmHg (no= 0; yes= 1)
    - c. ED heart rate greater than 120 bpm (no= 0; yes= 1)
    - d. Positive Ultrasound FAST Exam (no= 0; yes= 1)
  - 5. Trauma patient who requires more than 1 liter crystalloid to maintain systolic blood pressure greater than 90mmHg.

# Responsible Parties

- A. Team leaders: depending on area in hospital
  - 1. Trauma surgeon (trauma bay, operating room (OR), intensive care unit (ICU))
  - 2. Intensivist (in ICU when trauma surgeon unavailable).
  - 3. ED physician (in ED when trauma surgeon unavailable)
  - 4. Anesthesiologist (in OR or Post Anesthesia Care Unit (PACU))
  - 5. Trauma advanced practice provider (APP)
  - 6. Obstetrician (OB)
  - 7. Sound hospitalist
- B. Clinical pathologist
- C. Lab blood bank / laboratory personnel
- D. Pharmacy
- E. Nursing supervisor / charge nurse
- F. Clinical team:
  - 1. Trauma physician assistant (PA)/nurse practitioner (NP)
  - 2. ED registered nurse (RN)/paramedic
  - 3. ICU RN
  - 4. OR RN
  - 5. ED Technician / ICU technician / OR technician
- G. Vascular Access

# Procedure

- A. Initiation of the massive transfusion protocol (MTP):
  - 1. Trauma surgeon, intensivist, ED physician, trauma APP, anesthesiologist, Sound hospitalist, or OB initiate MTP.
    - a. Staff member call switchboard to page out MTP overhead and to all responsible parties.
    - b. Staff member enter order for Massive Transfusion in Cerner
      - i. Initiate *Lab - every 30 minutes* immediately
    - c. Blood bank and lab supervisor notified (by switchboard) of MTP initiation.
    - d. Nursing/house supervisor to come to area if needed.
    - e. Blood bank will notify clinical pathologist of MTP initiation
    - f. Maintain communication with blood bank during the initiation and maintenance of MTP.



delivered. This should prevent inappropriate temperature storage of a blood product, such as refrigeration of platelets.

- f. Prepares trauma packs (see attached schedule). Trauma packs should be ready to be delivered every 20 minutes.
- g. Updates to appropriate type-specific or crossmatched components once available.
- h. Tracks results of labs as they become available.
- i. Communicates with clinical pathologist and designated clinical team leader (usually the trauma surgeon, anesthesiologist, or intensivist depending on clinical area).
- j. Access and maintenance of services:
  - i. Notifies blood center and requests urgent delivery as needed.
  - ii. Communicates status of reserves to clinical pathologist.

5. ED RN/paramedic and ICU RN respond to all MTPs

- a. Maternity Unit: ED Brings Belmont and Maternity provides the MTP Cart
- b. ED MTP: ICU brings the Belmont only (not the MTP cart)
- c. All Other Units: ICU Brings MTP Cart and Belmont. ED also brings Belmont for backup.

6. Vascular Access ensure patient has large bore IV (unless physician inserting Cordis)

B. Maintenance of MTP:

1. Charge nurse/Patient Care Coordinator:

- a. Checks for accuracy of specimens and verification of patient identity.
- b. Expedites transfer of patient within the institution.
- c. Expedites transfer of lab specimens in timely fashion.
- d. Communicates with and assists clinical team to maintain accuracy and timeliness.

2. Clinical team:

- a. Draws, labels and maintains serial labs every 30 minutes during MTP or until discontinued by team leader (see heading III, below).
- b. Transfuses shipped trauma packs at regular intervals as needed
- c. Documents Input/Output (I/O) and medication administration record (MAR) during MTP.
- d. Accompany the patient to the OR or ICU.
- e. Remain with the patient until the MTP is terminated.

3. Team leader:

- a. Ensures timeliness of serial blood draws.

- b. Ensures timeliness of transfusions.
- c. Supervises clinical team during the maintenance of MTP.
- d. Designates alternate team leader when appropriate (e.g.: trauma surgeon designates anesthesiologist when operating).
- e. Communicates with clinical pathologist regarding trend of lab results and transfusion needs.

- i. Laboratory goals:

- 1. HGB 8-10 g/dL during the resuscitation and in the first 24 hours post stabilization. After 24 hour period of stabilization the HGB may be reduced to 7 g/dL if not actively bleeding.
- 2. Platelet count greater than 100,000 during resuscitation and in the first 24 hours post stabilization. After the 24 hour period of stabilization the goal is a platelet count greater than 50,000.
- 3. Coagulation testing goals: INR less than 2.0 and PTT less than 55 seconds. INR of 1.8 may be needed in TBI patients.
- 4. Fibrinogen greater than 150 mg/dL.

- f. Terminates MTP (See heading III)

- 4. Clinical pathologist or designee:

- a. Monitors coagulation and lab results
- b. Advises team leader and clinical team of need for other blood components or specific alterations in transfusion needs (e.g. cryoprecipitate)
- c. Notifies team leader of critical shortages in blood supply.

C. Termination of MTP:

- 1. Determined by team leader when either of the following are achieved
  - a. Achievement of endpoints of resuscitation ("stabilization").
    - i. Normalization of vital signs, including temperature.
    - ii. Normalization or improvement of coagulation parameters.
    - iii. Termination of bleeding/exsanguination.
  - b. Failure or Futility.
- 2. Call 55555 for switchboard to announce termination of MTP overhead.
- 3. Maintenance of hematologic function:
  - a. Serial hematologic assessments (CBC, PT/INR, PTT) every 6 hours for 24 hours, then twice daily (BID) or as needed.
  - b. Do not transfuse if there is no evidence of bleeding

- c. Transfuse FFP if there is evidence of oozing until INR less than 2.0.
  - d. Transfuse platelets if platelets less than 50 k/dL.
  - e. Transfuse red blood cells (RBC) to maintain HGB 8-10 g/dL in first 24 hours post stabilization; transfuse for **HGB** less than 7 g/dL after 24 hours (restrictive transfusion trigger) unless evidence of new bleeding.
  - f. Transfuse cryoprecipitate if fibrinogen less than 150 g/dL.
- D. Review of case and debriefing:
- 1. What went well.
  - 2. What did not.
  - 3. Product wasted.
- E. \*If rotational thromboelastometry (ROTEM) is available, the following cut-points for transfusion triggers may also be used:
- 1. Plasma for CT exTEM greater than 100 seconds and/or CT inTEM greater than 230 seconds.
  - 2. Cryoprecipitate (fibrinogen concentrate) and/or plasma for MCF fibTEM less than 8 mm.
  - 3. Platelets for MCF exTEM less than 45 mm and MCF fibTEM greater than 10 mm.
  - 4. Anti-fibrinolytics for ML exTEM greater than 15 percent.

Document ID: 038.P003

COPY

## Attachments

- [ED Step-by-step instructions for using the Massive Transfusion Protocol Edits.doc](#)
- [Expected Response to Product](#)
- [MTP schedule.docx](#)
- [Step by step instructions for MTP in ICU 2019.pdf](#)

## Approval Signatures

Step Description	Approver	Date
System Policy Oversight Committee	Terri Fries: Document Mgmt Spec	5/15/2023

Mgr Trauma Program

Sarah Helveston: Mgr Trauma  
Program

5/15/2023

Document Owner

Kerry Kole: Medical Director

5/13/2023

---

## Applicability

Munson Medical Center

## Standards

No standards are associated with this document

COPY